


NOTES:

1. FLANGE MATERIAL-ALUMINIUM
TERMINAL MATERIAL-BRASS
2. TAPER AND CONTACTS TO MATE WITH 350KV ESSEX
STANDARD TERMINATION WITH WIDE BAND TIPS
3. MATERIAL OF INSULATION TO BE CAPABLE OF
CONTINUOUS IMMERSION IN SHELL DIALA BG OIL &
▲ SF6 AT 75PSI G
4. SEE SHEET TWO FOR INTERNAL DIMS

SURFACE ROUGHNESS
ALL MACHINE SURFACES 3.2Ra
UNLESS OTHERWISE STATED

FINISH
REMOVE BURRS & SHARP EDGES
DE-GREASED

ESSEX Essex X-Ray & Medical Equipment LTD Registered Office Fitch Industrial Estate Chelmsford Road Dunmow Essex CM6 1XJ Telephone 01371 875661 Fax 01371 875665	REVISIONS		TOLERANCE	DRAWN DJM	MATERIAL SEE NOTES	
	No.	DATE	BY	1dp ± 0.3		CHECKED <i>MJ</i>
	2	19.02.14	DCN 3940	2dp ± 0.1	APPROVED <i>[Signature]</i>	CONCENTRICITY 0.1 TIR
				Δ $\pm 0.5^\circ$	DATE 22.08.13	ISSUE 2
				TITLE	SCALE 1:1 @ A3	DRAWING No.
				350 KV GEN RECEPTACLE EXTENDED LENGTH, WIDE BAND		T22498

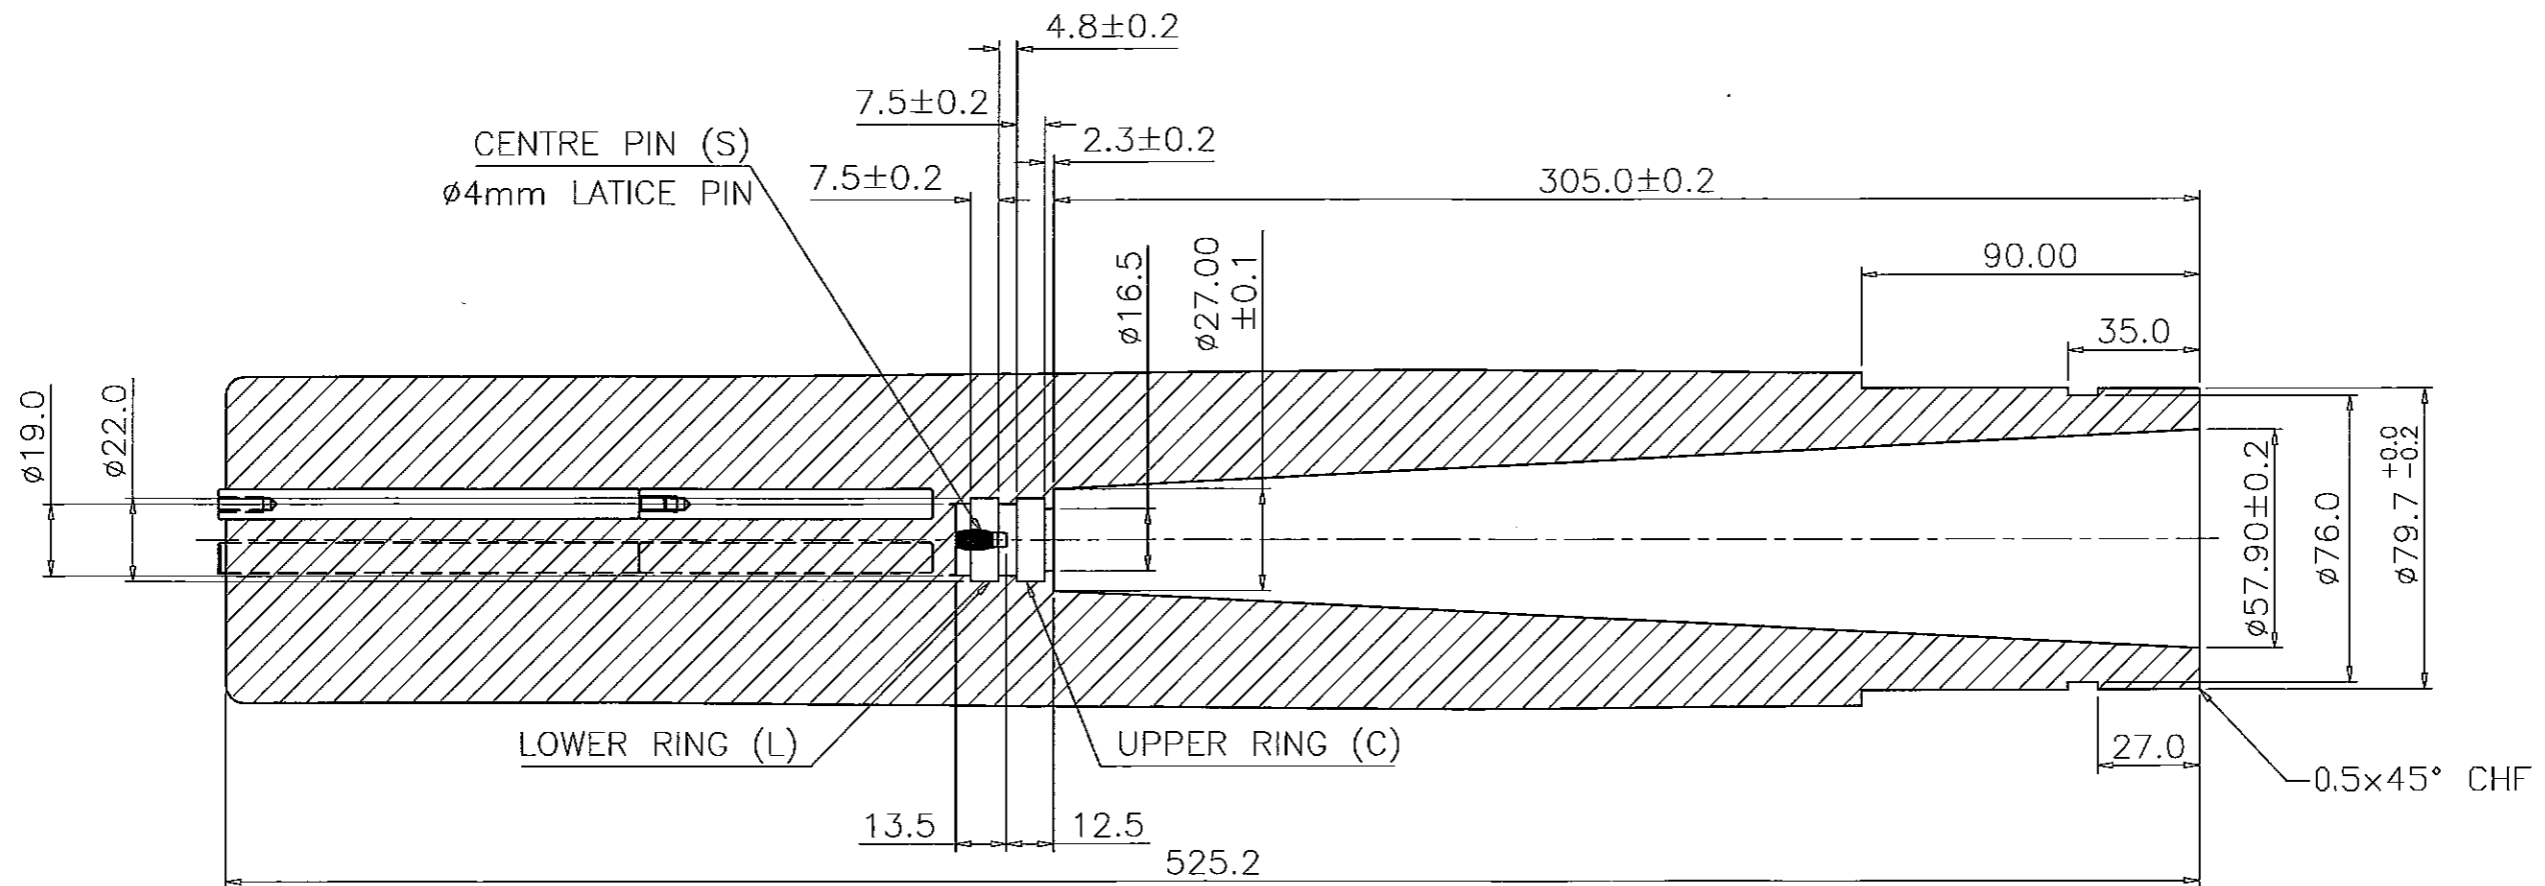

NOTES:
1. SEE SHEET ONE FOR EXTERNAL DIMENSIONS

SURFACE ROUGHNESS
ALL MACHINE SURFACES 3.2Ra
UNLESS OTHERWISE STATED

FINISH
REMOVE BURRS & SHARP EDGES
DE-GREASED

<p>ESSEX</p> <p>Essex X-Ray & Medical Equipment LTD</p> <p>Registered Office: Flitch Industrial Estate, Chelmsford Road, Dunmow Essex CM6 1XJ Telephone: 01371 875661, Fax: 01371 875665</p>	REVISIONS			TOLERANCE	DRAWN DJM	MATERIAL EPOXY RESIN
	No.	DATE	BY	1dp ±0.3	CHECKED <i>MS</i>	
	2	19.02.14	DCN 3940	2dp ±0.1	APPROVED <i>[Signature]</i>	DATE 22.08.13
				±0.5°		ISSUE 2
					TITLE	SCALE 1:2 @ A3
					350KV GEN RECEPTACLE EXTENDED LENGTH, WIDE BAND	DRAWING No. T22498