



Conceptual Design of Compact Photon Source for KLF

Hovanes Egiyan

Pavel Degtiarenko


Overview

- Requirements for CPS
- Model Description
- Photon Beam from CPS
- Radiation Environment
- Temperature in CPS absorber
- Electron Beam Requirements for CPS
- Summary



Introduction

- KLF experiment needs to produce high intensity photon beam for KPT.
- CPS stands for Compact Photon Source; it has been proposed as the photon source.
- The only possible location for such a source is the Tagger Hall.
- CPS beamline will require major modifications to GlueX photon beamline.

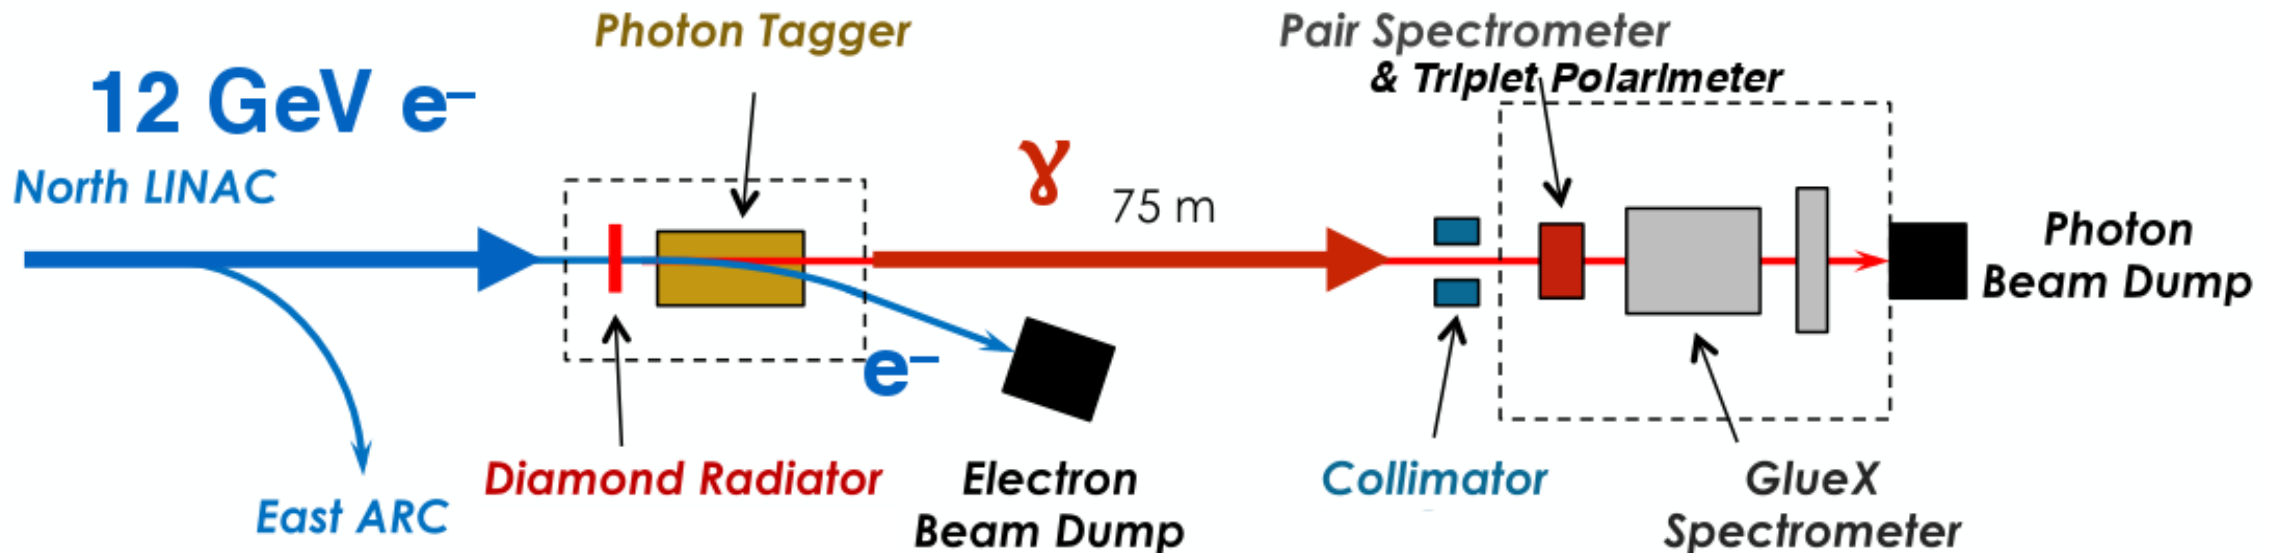

Review Charge Items

- Is there any R&D needed to be done prior to start the construction of the Klong Facility?
- What is the status of the Compact Photon Source (CPS)? Specifically:
 - a) the conceptual design
 - b) the evaluation of the produced radiation. In particular, the following points should be discussed:
 1. the approximations made in the Monte Carlo simulations and which code has been used;
 2. the energy deposition and the absorber temperature;
 3. the prompt dose and activation around the CPS and the Tagger Hall;
 4. the magnet performance and its coils lifetime;
 5. ~~the water cooling system and possible contaminations.~~
- Will civil constructions be needed to contain the radiation in the Tagger Hall?
- What will the photon beam quality be?
- What are the requirements of the electron beam on the CPS?
- What is the decommissioning plans for the K-Long Facility (CPS, KPT,...) and the activated components? A brief outline is sufficient.




CPS Requirements

- Intense photon flux of $\Phi_\gamma > 10^{12}$ photons per second with $1.5 \text{ GeV} < E_\gamma < 12 \text{ GeV}$.
- Photon beam spot size at KPT with $2 \cdot \Gamma_\gamma < 6 \text{ cm}$ to make full use of KPT size.
- Radiation environment in the Tagger Hall similar or better than what GlueX would get with 5 μA electron beam on nominal GlueX diamond radiator.
 - ❑ Prompt dose rate equivalent of $\sim 20 \text{ rem/hr}$.
 - ❑ Activation dose rate $< 5 \text{ rem/hr}$ after 1000 hours of operations and 1 hour of cool-down time.
 - ❑ RadCon limits $< 1 \text{ mrem/hr}$ outside of the Tagger Hall.
- Cooling system design that is sufficient to handle $\sim 54 \text{ kW}$ power delivered to CPS.
 - ❑ It will need to be closed-circuit system to avoid activation/contamination.
- GlueX beamline should be restored relatively quickly without disassembly of CPS.
 - ❑ GlueX photon beamline is wider than CPS beam channel and is under vacuum.
 - ❑ We decided to build a movable platform to move CPS beam-left.



CPS Positioning in the Hall D Tagger

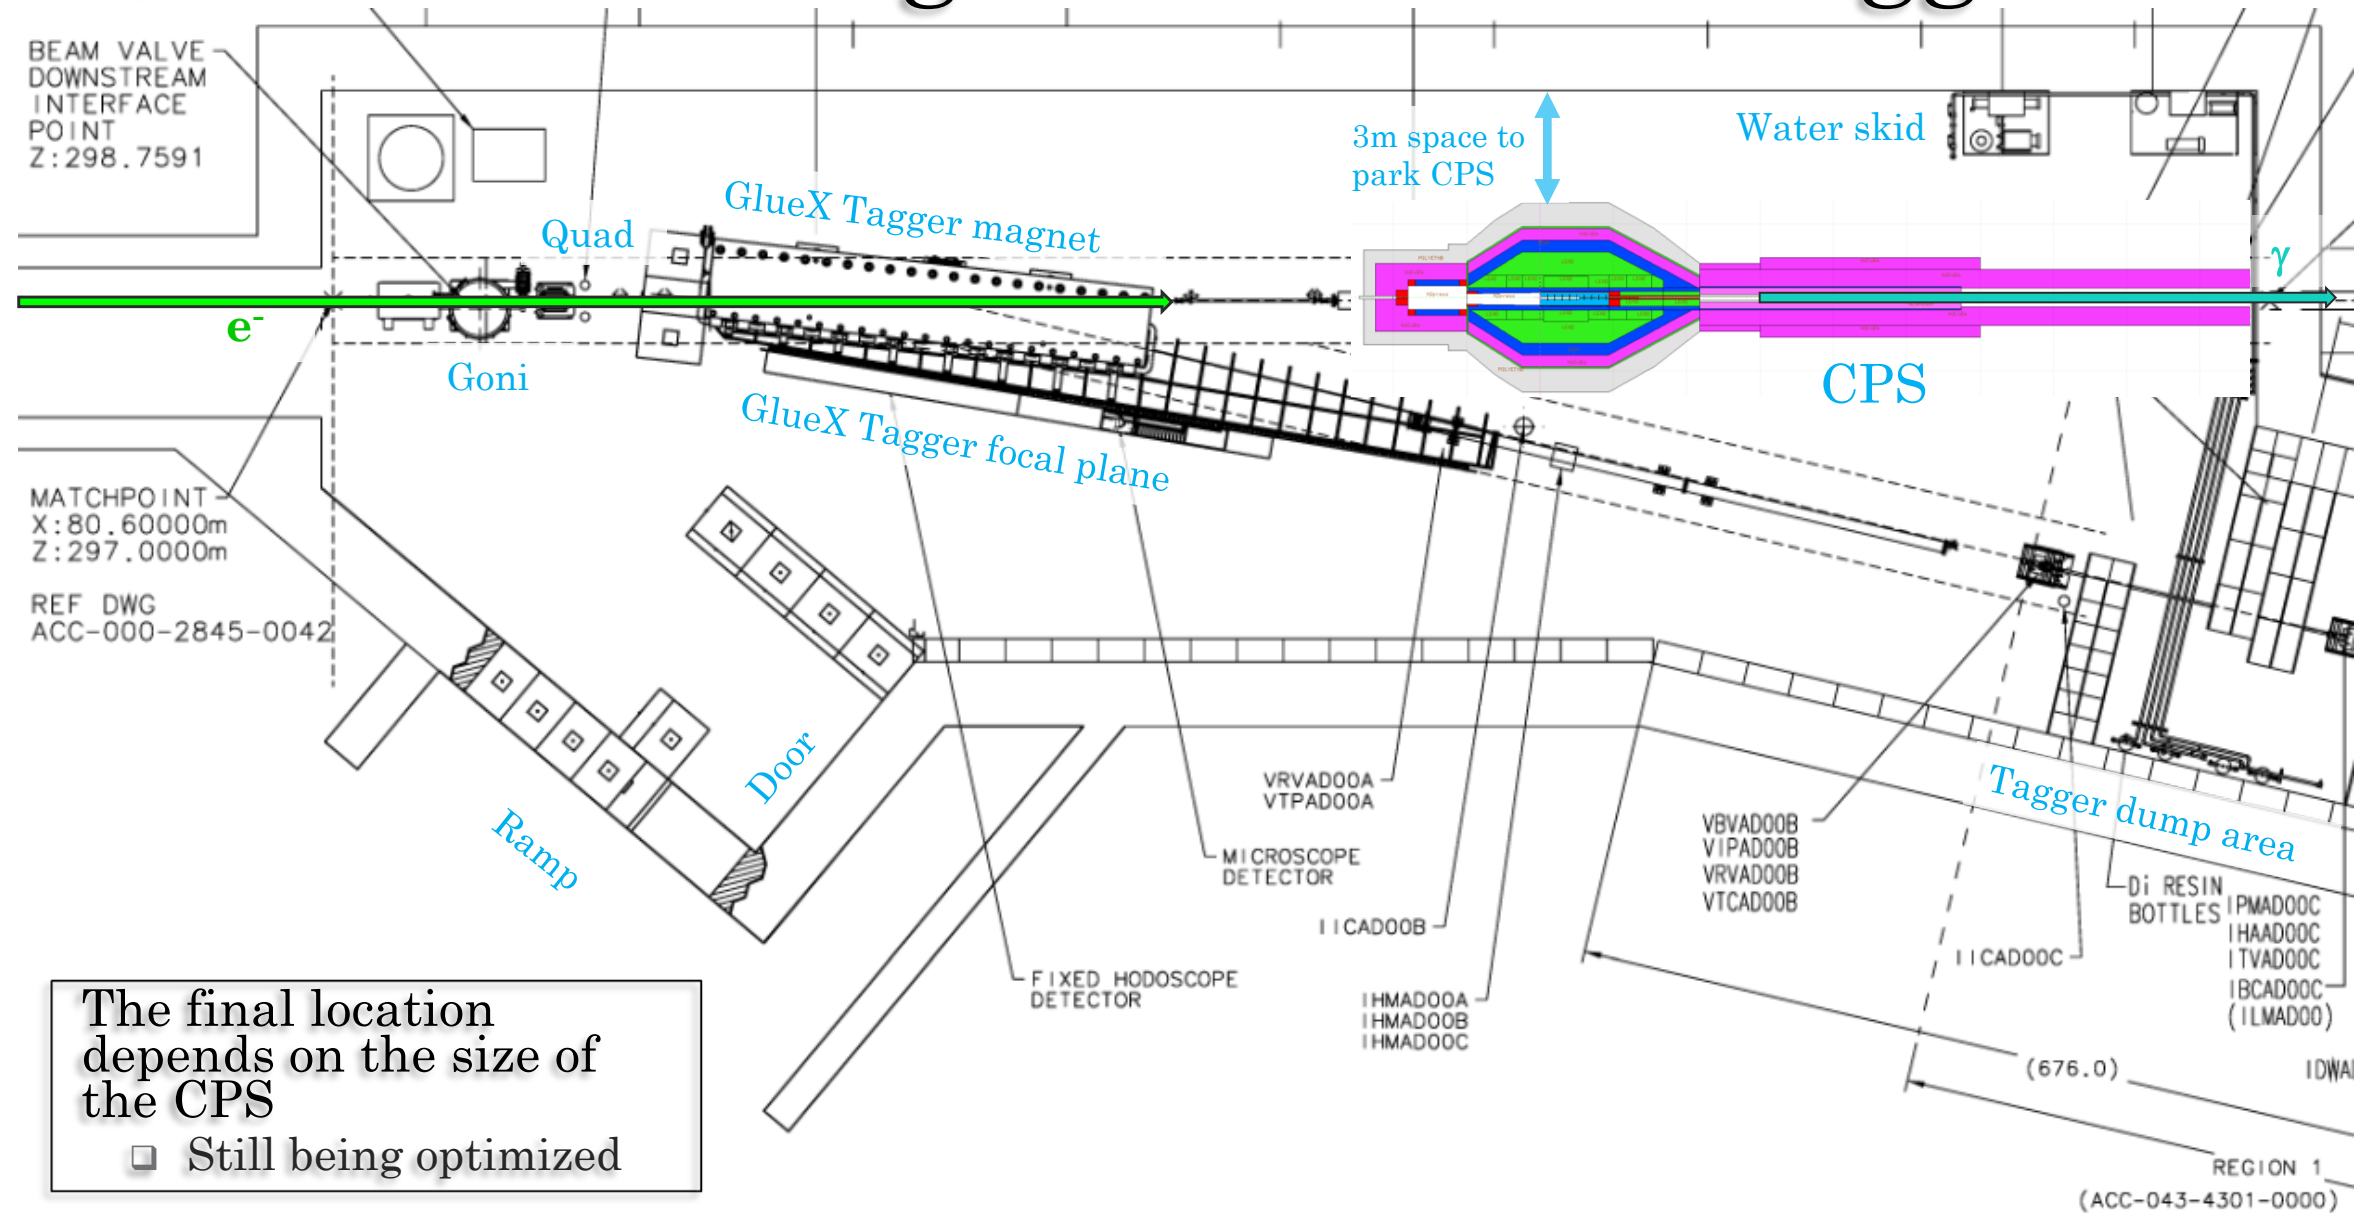

The final location depends on the size of the CPS

- Still being optimized

Hall D Design Development


- We started with Hall C version of the CPS.
 - ❑ Very compact design
 - Small footprint in the hall.
 - The radiator, magnet, and the absorber are in the same region.
 - High power deposition densities leading to high temperatures in the core.
 - Requires a magnet with high magnetic field $B > 3$ Tesla.
 - ❑ Costs \$2M or more mainly due to the use of tungsten as shielding material.
- Considered two different models with lower magnet field during last year.
 - ❑ Vitaly Baturin developed a model in the summer of 2022.
 - ❑ Pavel Degtiarenko proposed another model in the fall of 2022.
 - ❑ After studying both models, we chose one for further optimization and engineering design.
- Currently we are in the process of optimizing the design.
- People involved in CPS design work:
 - ❑ Physicists: V. Baturin, P. Degtiarenko, H. Egiyan
 - ❑ Engineers: T. Whitlatch
 - ❑ We may recruit a mechanical engineer to work on engineering design in the fall.





Hall D CPS Model

- Magnet and the absorber are separated by 1 meter .
 - ❑ No heat load on the magnet poles and coils from the core.
 - ❑ Low radiation exposure to the magnet.
- Clean-up magnet downstream for charged particles.
 - ❑ Utilize the existing permanent magnet used in GlueX beamline.
- No tungsten is used in the CPS shielding.
 - ❑ We save cost by using lead instead.
 - ❑ Small amount of a tungsten-copper mix is used for shielding the beam channel and magnet coils.
- Total estimated weight of CPS is approximately 76 metric tons.
 - ❑ Includes downstream beamline shielding.
 - ❑ Movable platform will add more weight.
 - ❑ Tagger Hall should easily handle CPS weighing 100 tons.
- Estimated cost of the current design is ~\$1M for CPS
 - ❑ Upstream beamline instrumentation will be extra.
- Tim Whitlatch will discuss engineering and cost related aspects in detail.

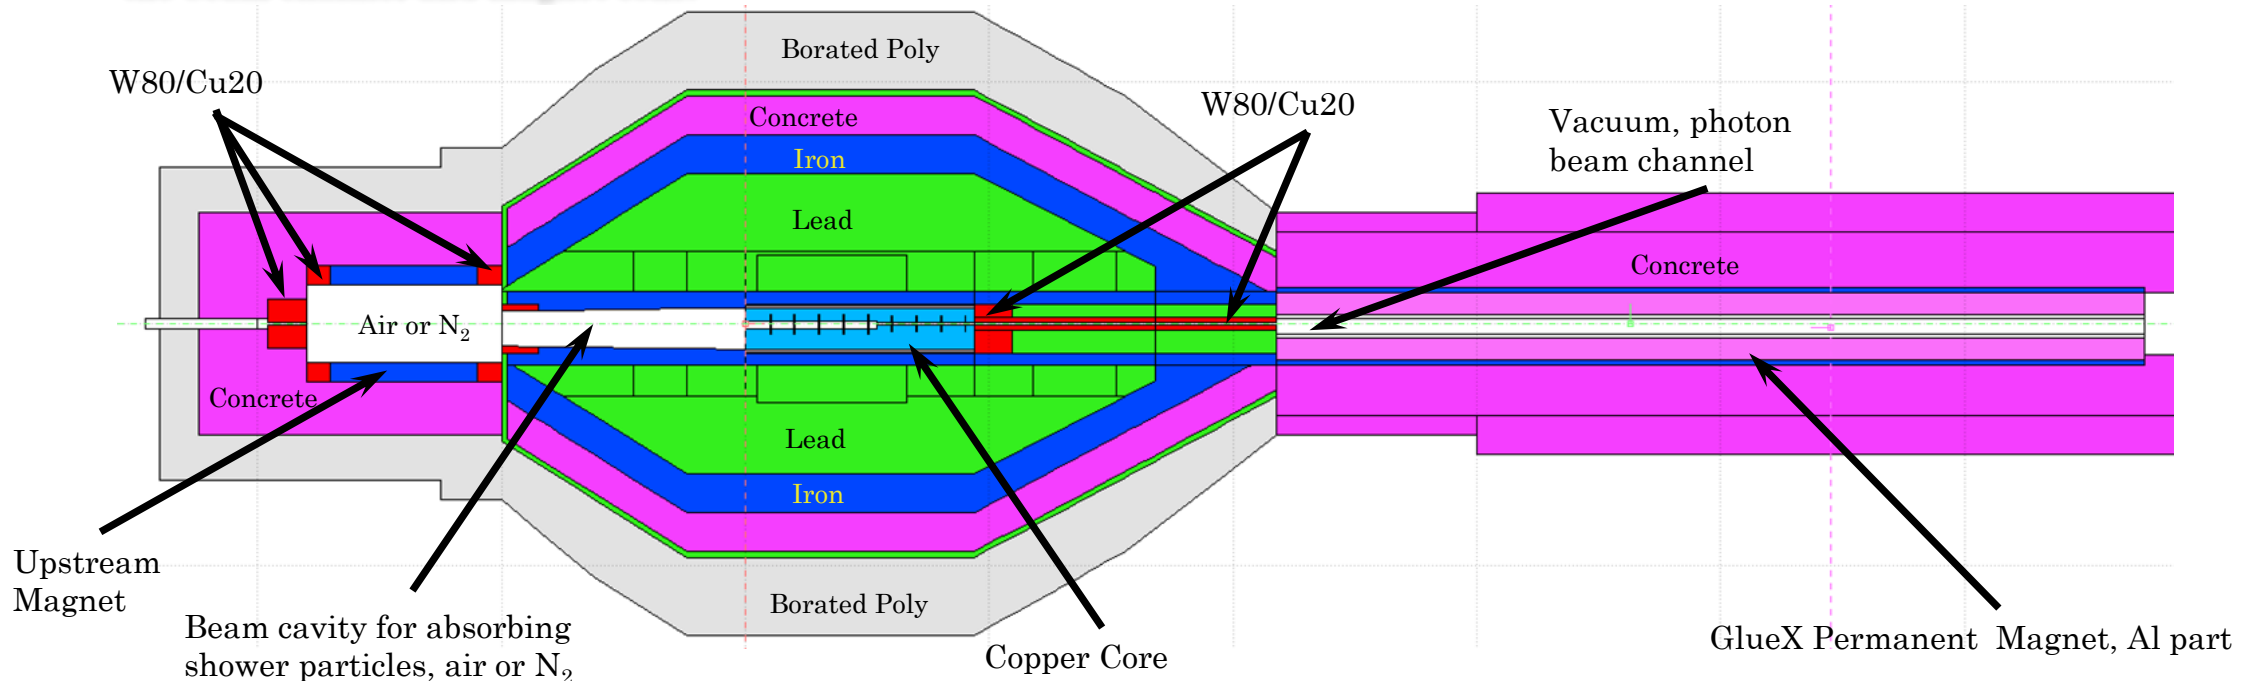



CPS Absorber

- Copper core with 20cm x 20cm x 94cm dimensions.
 - ❑ To absorb and dissipate the power.
 - ❑ Copper is not ferromagnetic and is a very good heat conductor.

- Varying size beam channel to trap the secondary particles from the electromagnetic shower.
 - ❑ Wider cavity upstream for trapping electrons and EM shower remnants.
 - ❑ Narrow conical channel with diameter ~1cm for outgoing photons.



- Cooling channels for water flow capable of evacuating ~54 kW power.

- Copper absorber is surrounded by air, steel, and W/Cu mix.
 - ❑ No contact with lead.

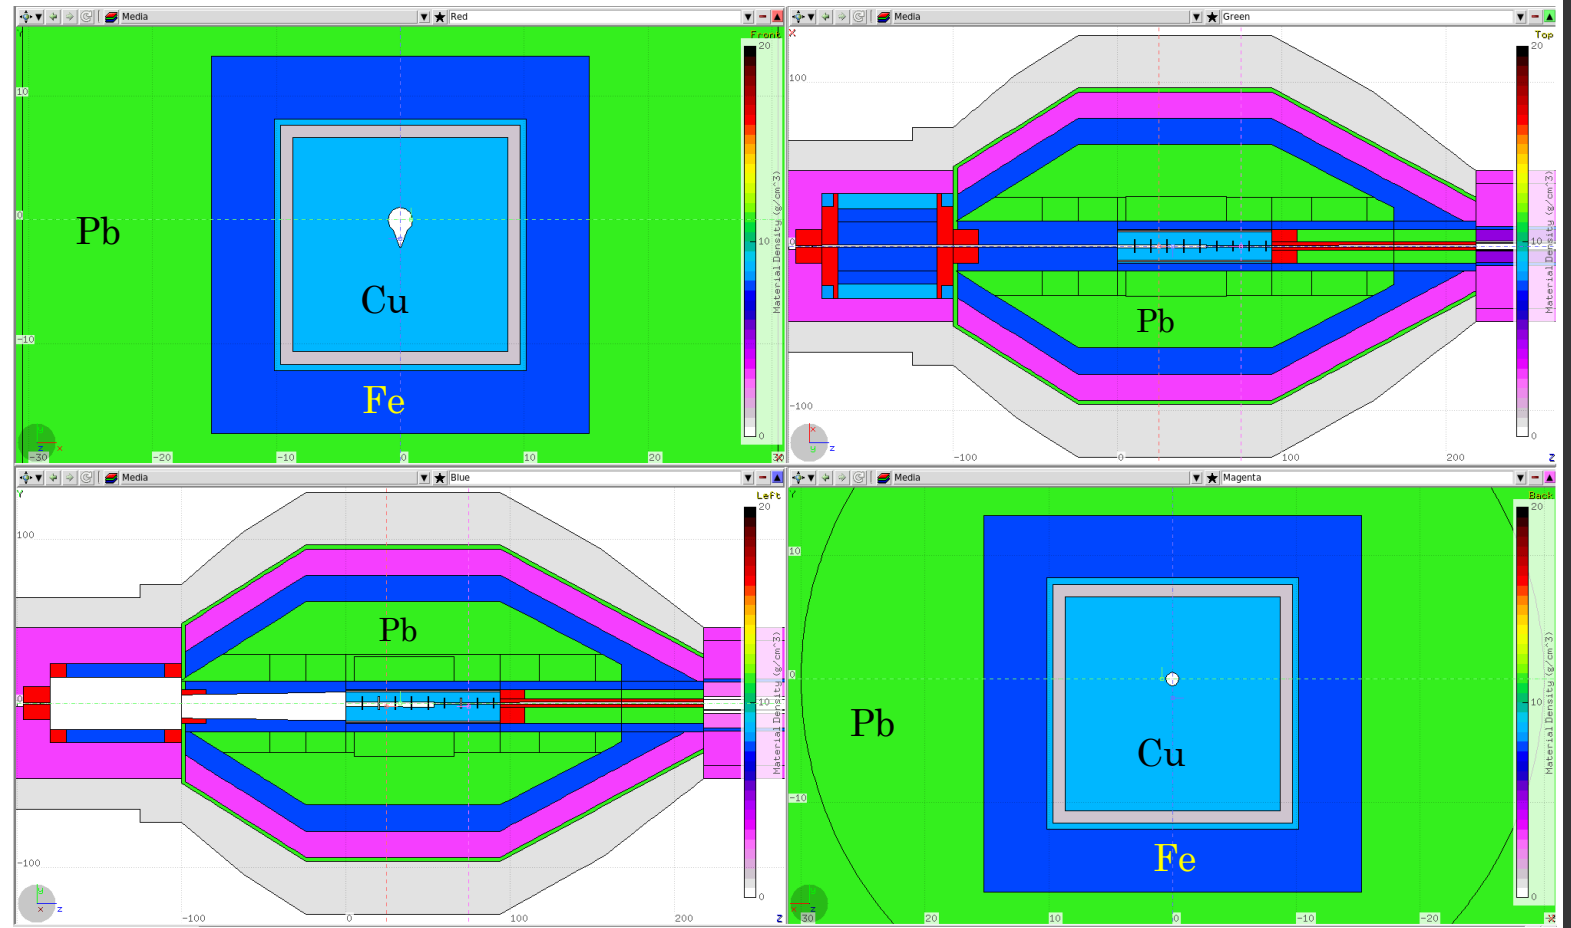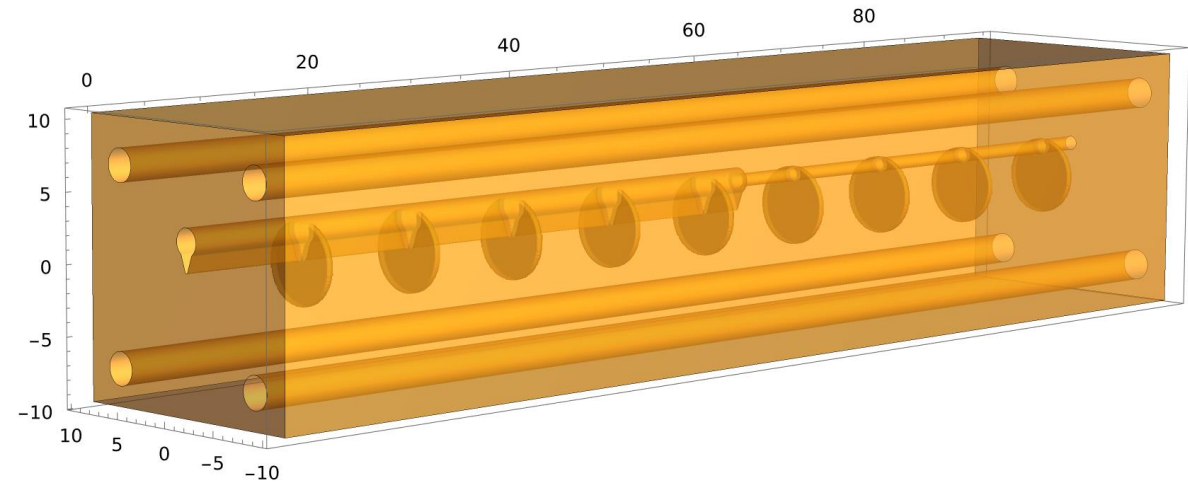

Upstream Magnet


- Current CPS design requires ~ 0.45 T·m magnetic field in the x-direction.
- We developed a draft model of the magnet.
 - ❑ Magnet has 60 cm long coils.
 - ❑ Bedstead shape of coils for less radiation exposure.
 - ❑ The closest distance from coils to the beam center is ~ 11 cm.
- The gap should be on the order 1 cm or more to avoid interaction with beam tails and halo.
 - ❑ Current design assumes 1.4 cm gap.
- Iron yoke with 8 cm thickness.
 - ❑ Total length of the yoke is 60cm
 - ❑ The transverse size of the yoke is 46cm x 48 cm.
- Chamfered iron poles.
- We used OPERA to calculate the field in the model.
 - ❑ The model can provide a dipole field of 0.67 T at 67 A/cm² current density in the coils.
 - Should be able to use Tagger Magnet power supply.
 - ❑ The field in the yoke is far from saturation point.
 - ❑ Field map is used in FLUKA simulations.

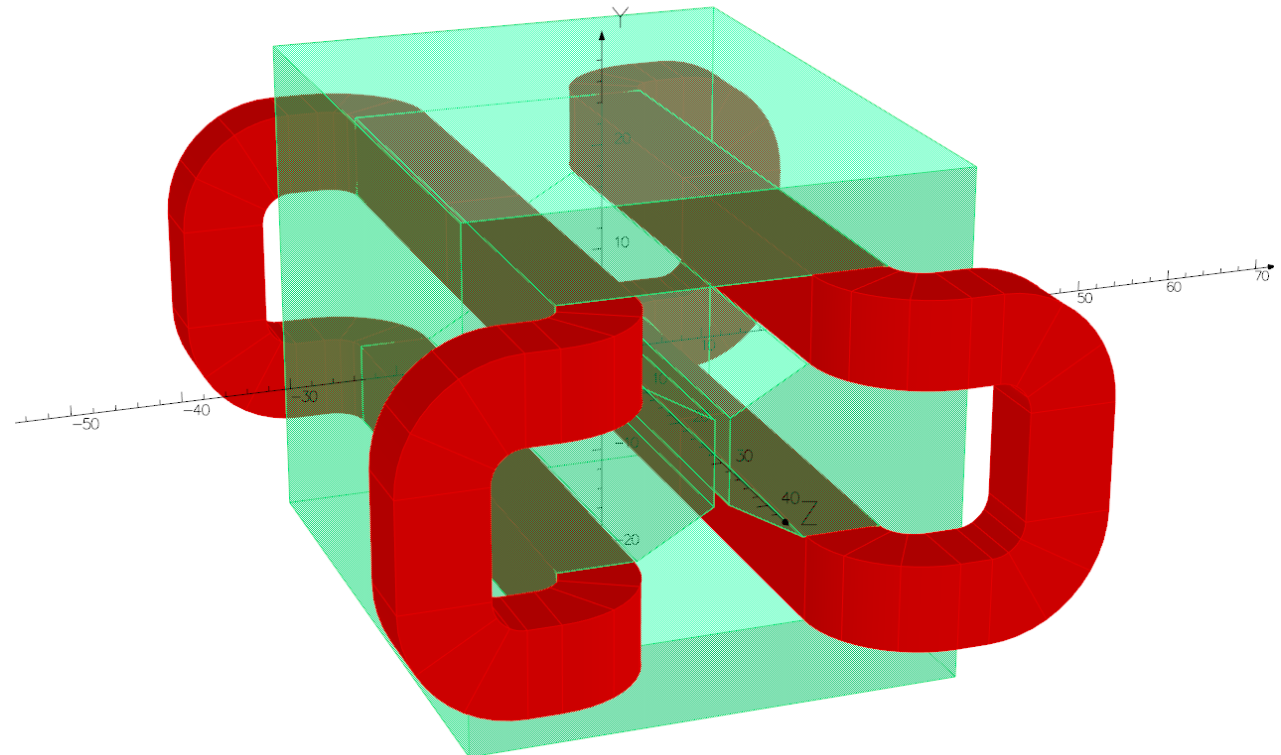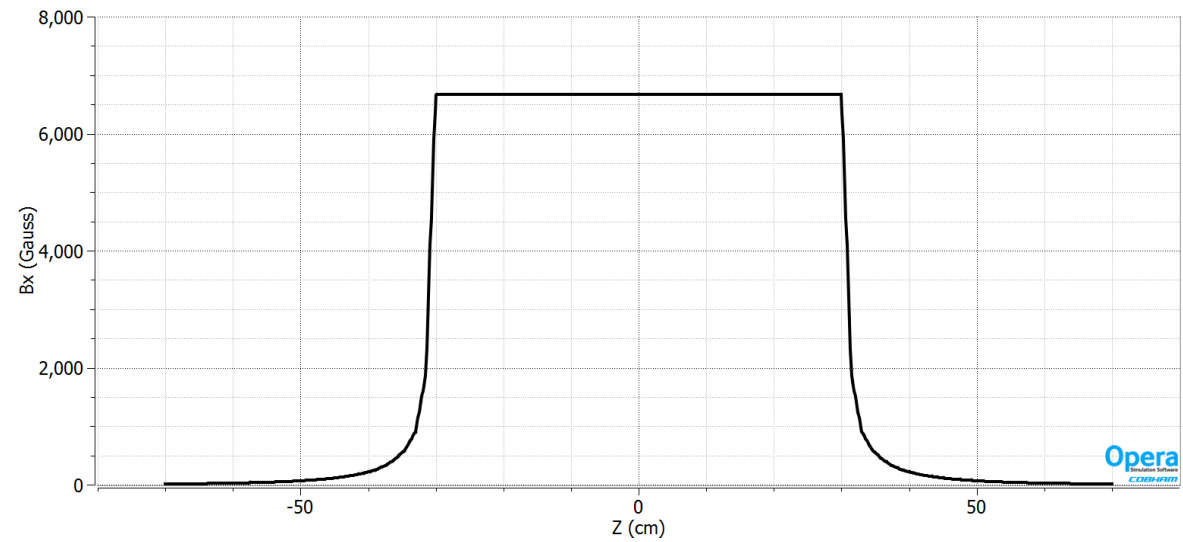

Downstream Magnet




- GlueX uses a 140" long permanent magnet from FNAL beamline to prevent electrons from leaking into the main hall.
 - ❑ Electron beam is interlocked to tagger magnet current at the power supply.
 - ❑ Leaks are only possible for short bursts when the tagger magnet trips.
 - ❑ KLF still needs it to prevent electron from accidentally penetrating to the hall.
- The magnetic material is made of strontium ferrite.
 - ❑ Can handle over 10^7 Gy radiation dose, according to the specs.
- Provides $\int B \cdot dL = 0.822 \text{ T}\cdot\text{m}$ field integral.
 - ❑ The exact field of this magnet is not important for CPS itself.
 - We use it to remove the charged particles from the photon beamline.

Cross section of the FNAL PDV magnet used by GlueX in the tagger hall.

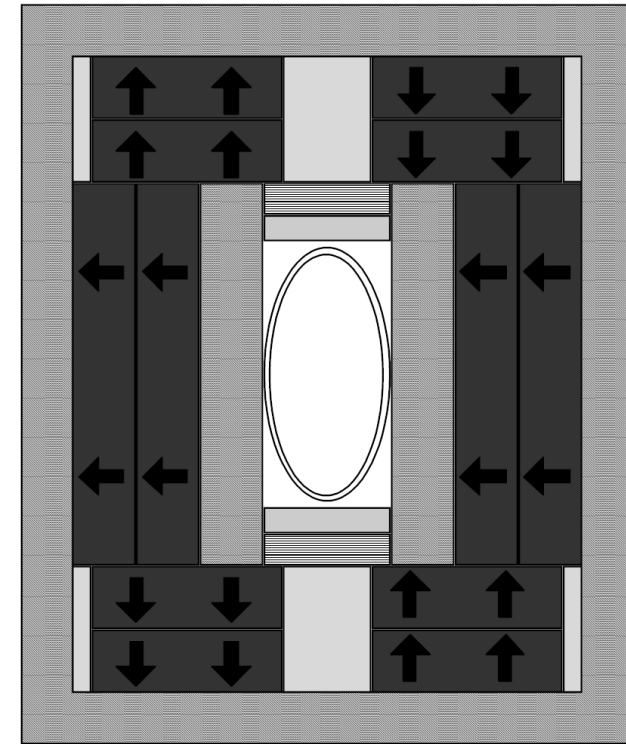




Photon Beam

- We used FLUKA to estimate the beam profile at KPT.
- Clean photon beam profile with $\sigma_\gamma \approx 1.5$ cm width.
 - ❑ The width is dominated by multiple scattering in the 10% radiator.
 - ❑ Vertical distribution has a slight asymmetry (on 0.1% level) favoring negative y-s.
- Charged particle and neutron rates from CPS measured at the KPT location is expected to be very small compared to the photon flux.

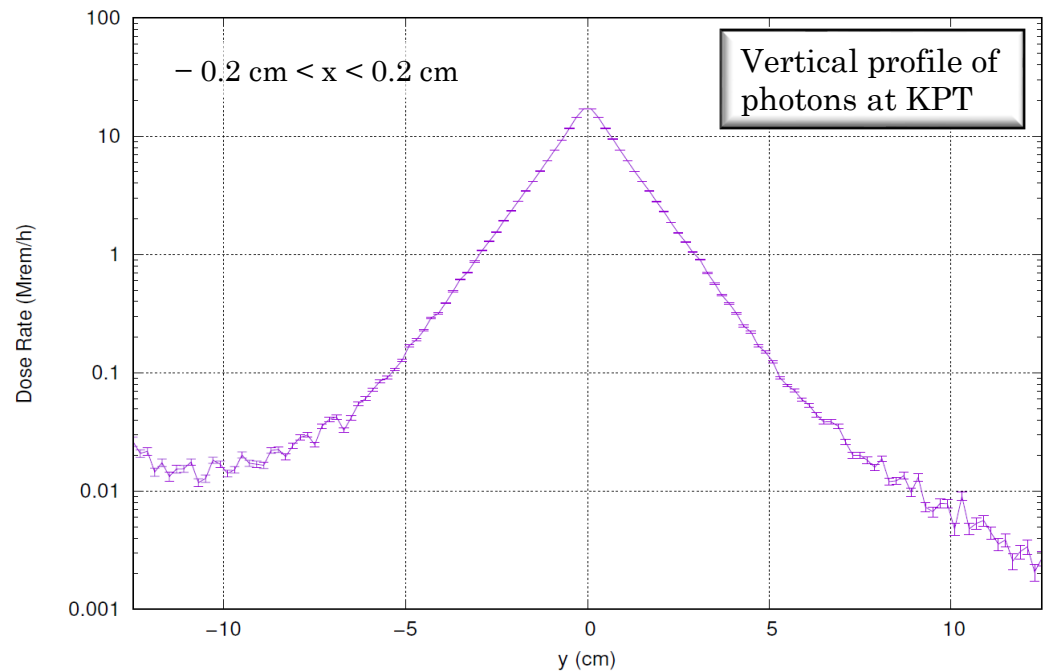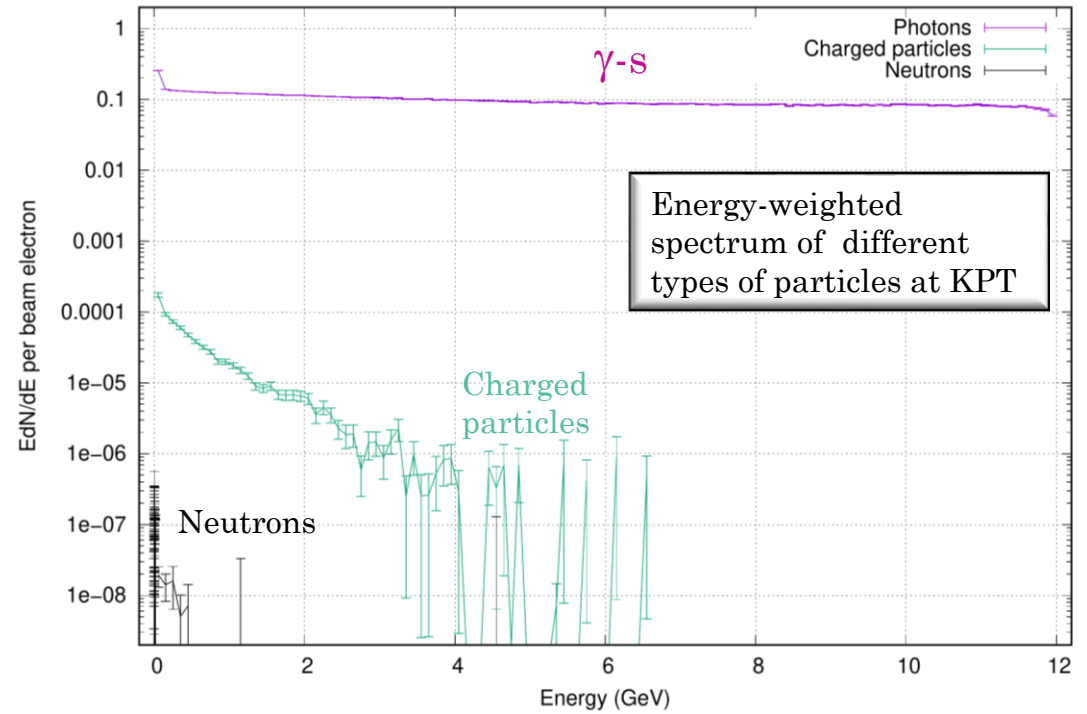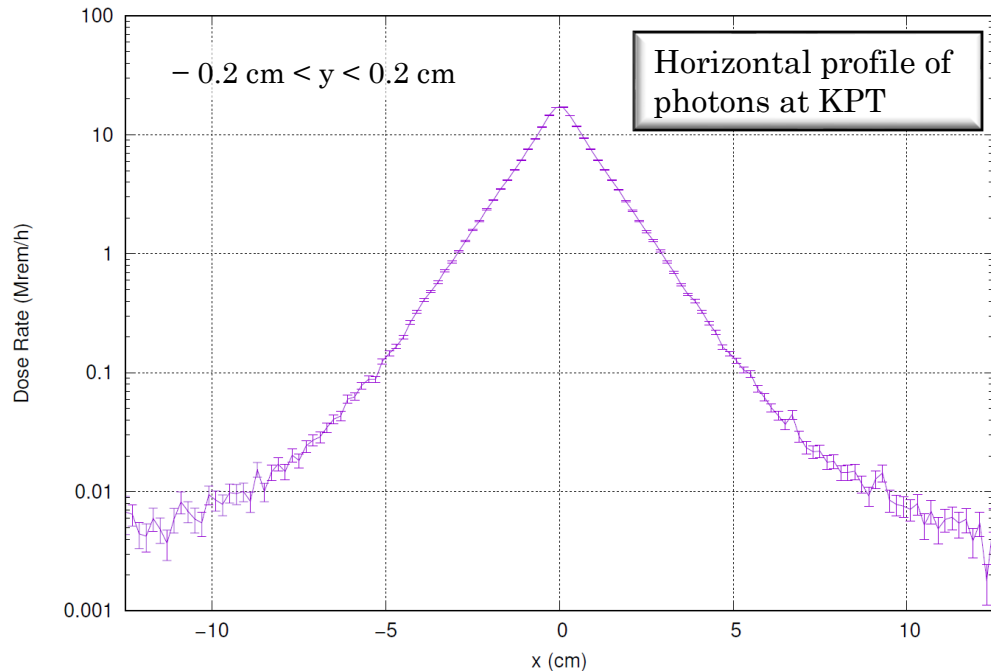


Prompt Dose Rates

- We estimated the prompt dose rates around the Tagger Hall.
 - ❑ More detailed simulation may need to be done.
- The results show that the rates on the surface of the berm will be below 1 mrem/hour.
 - ❑ No civil construction will be needed around Tagger Hall to contain radiation.
- The prompt dose rate around the 10" beam pipe between Tagger Hall and Collimator above the dirt is negligible.

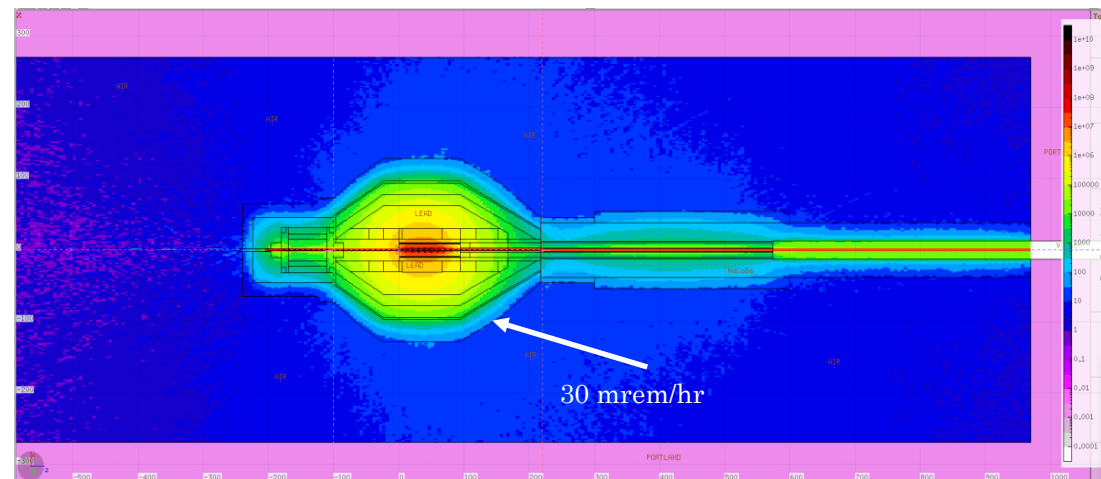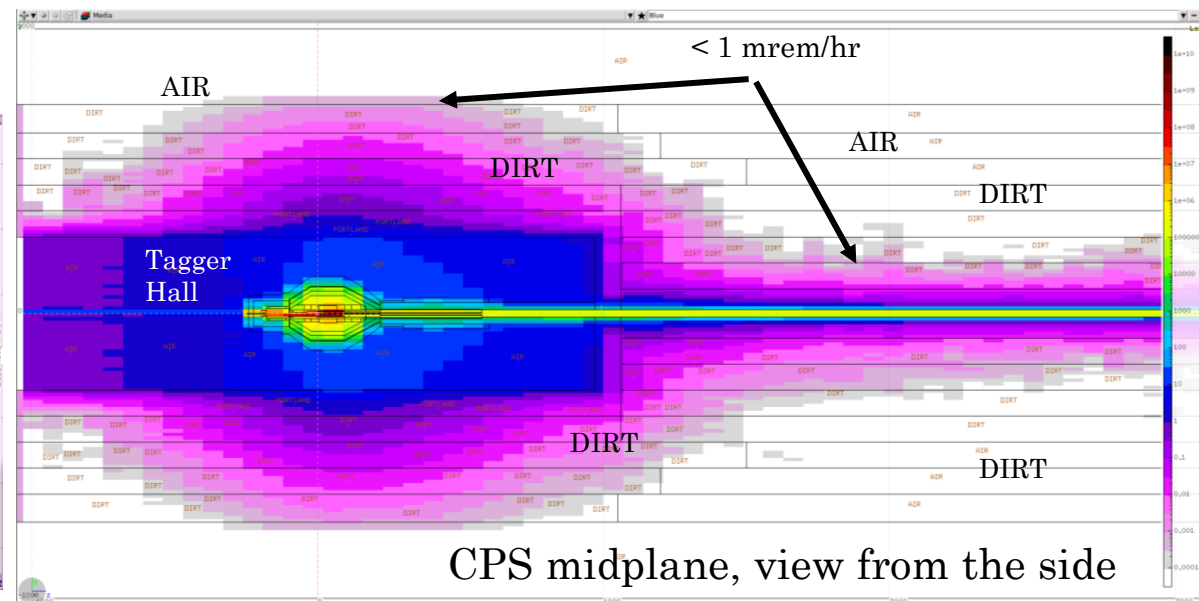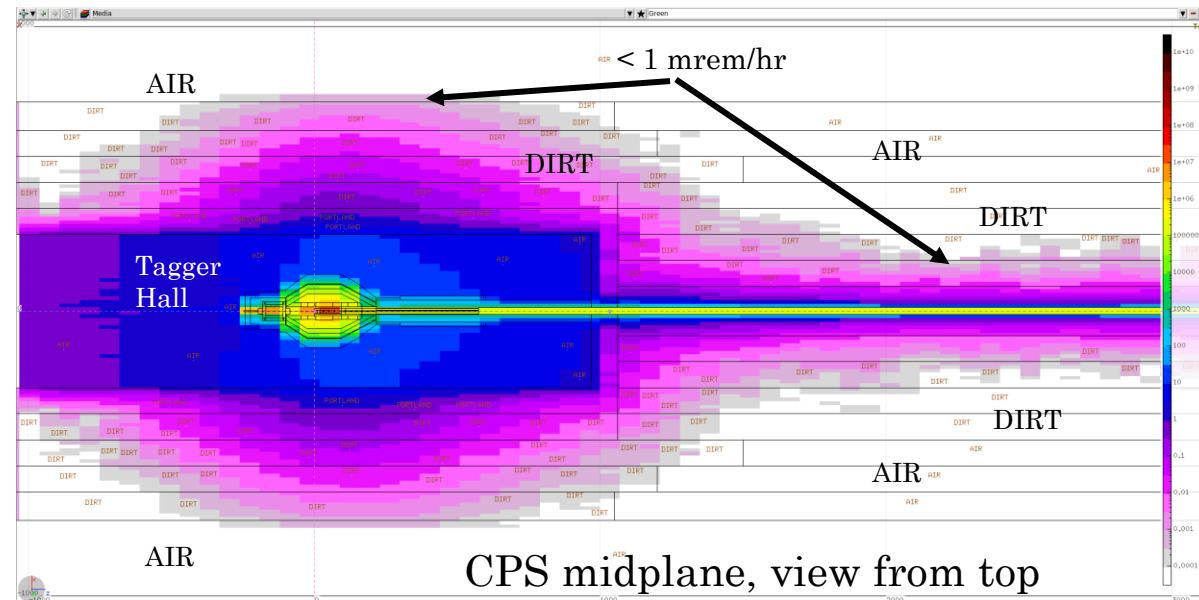


Activation Dose Rates

- We evaluated activation dose rate after 10000 hours of continuous operations and 1 hour cool-off time.
- The rates outside of CPS are expected to be 1rem/hr or below well within JLAB limits.

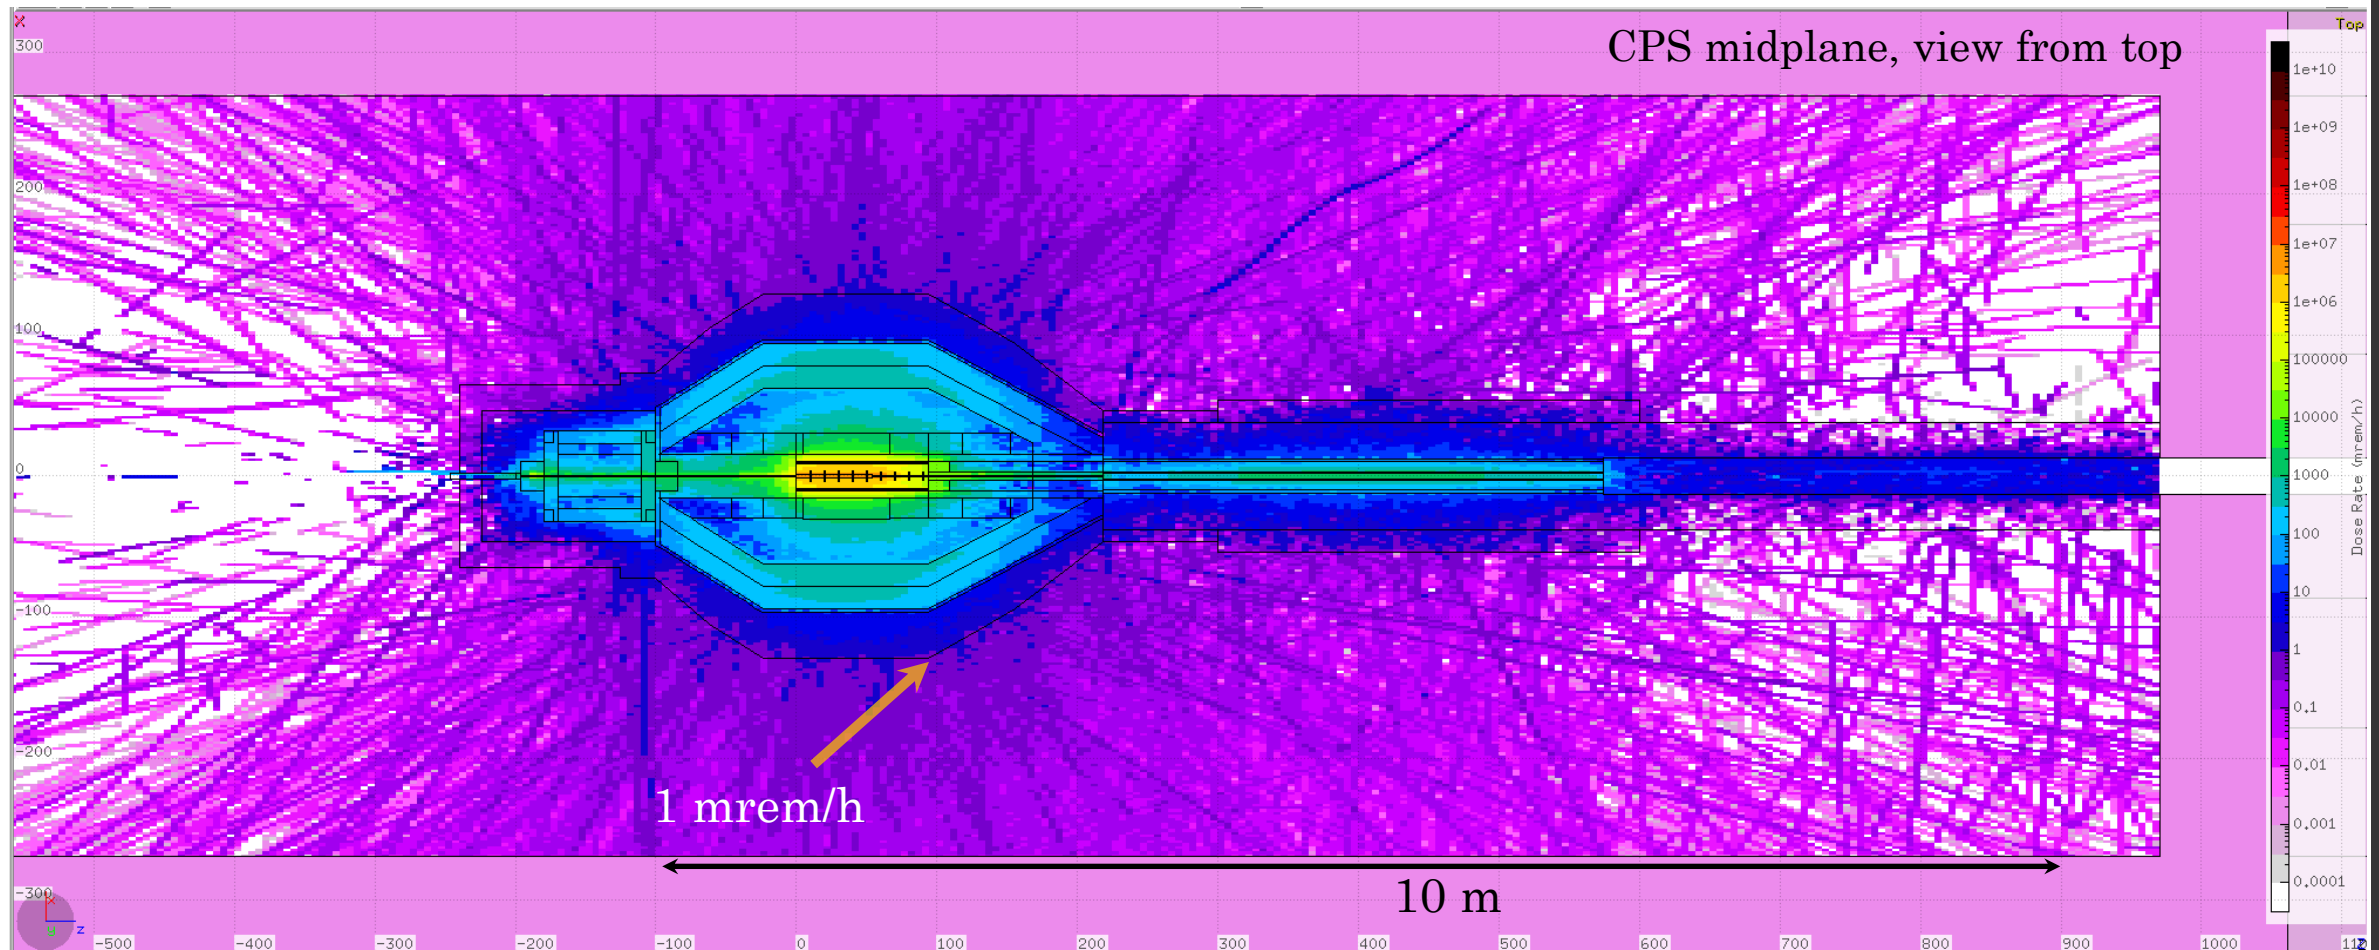

Accumulated Dose in 10000 hours



- Small accumulated doses are expected outside of CPS.
- CPS is not expected to be disassembled for a very long time.
 - ❑ It can be moved aside to restore GlueX photon beamline.

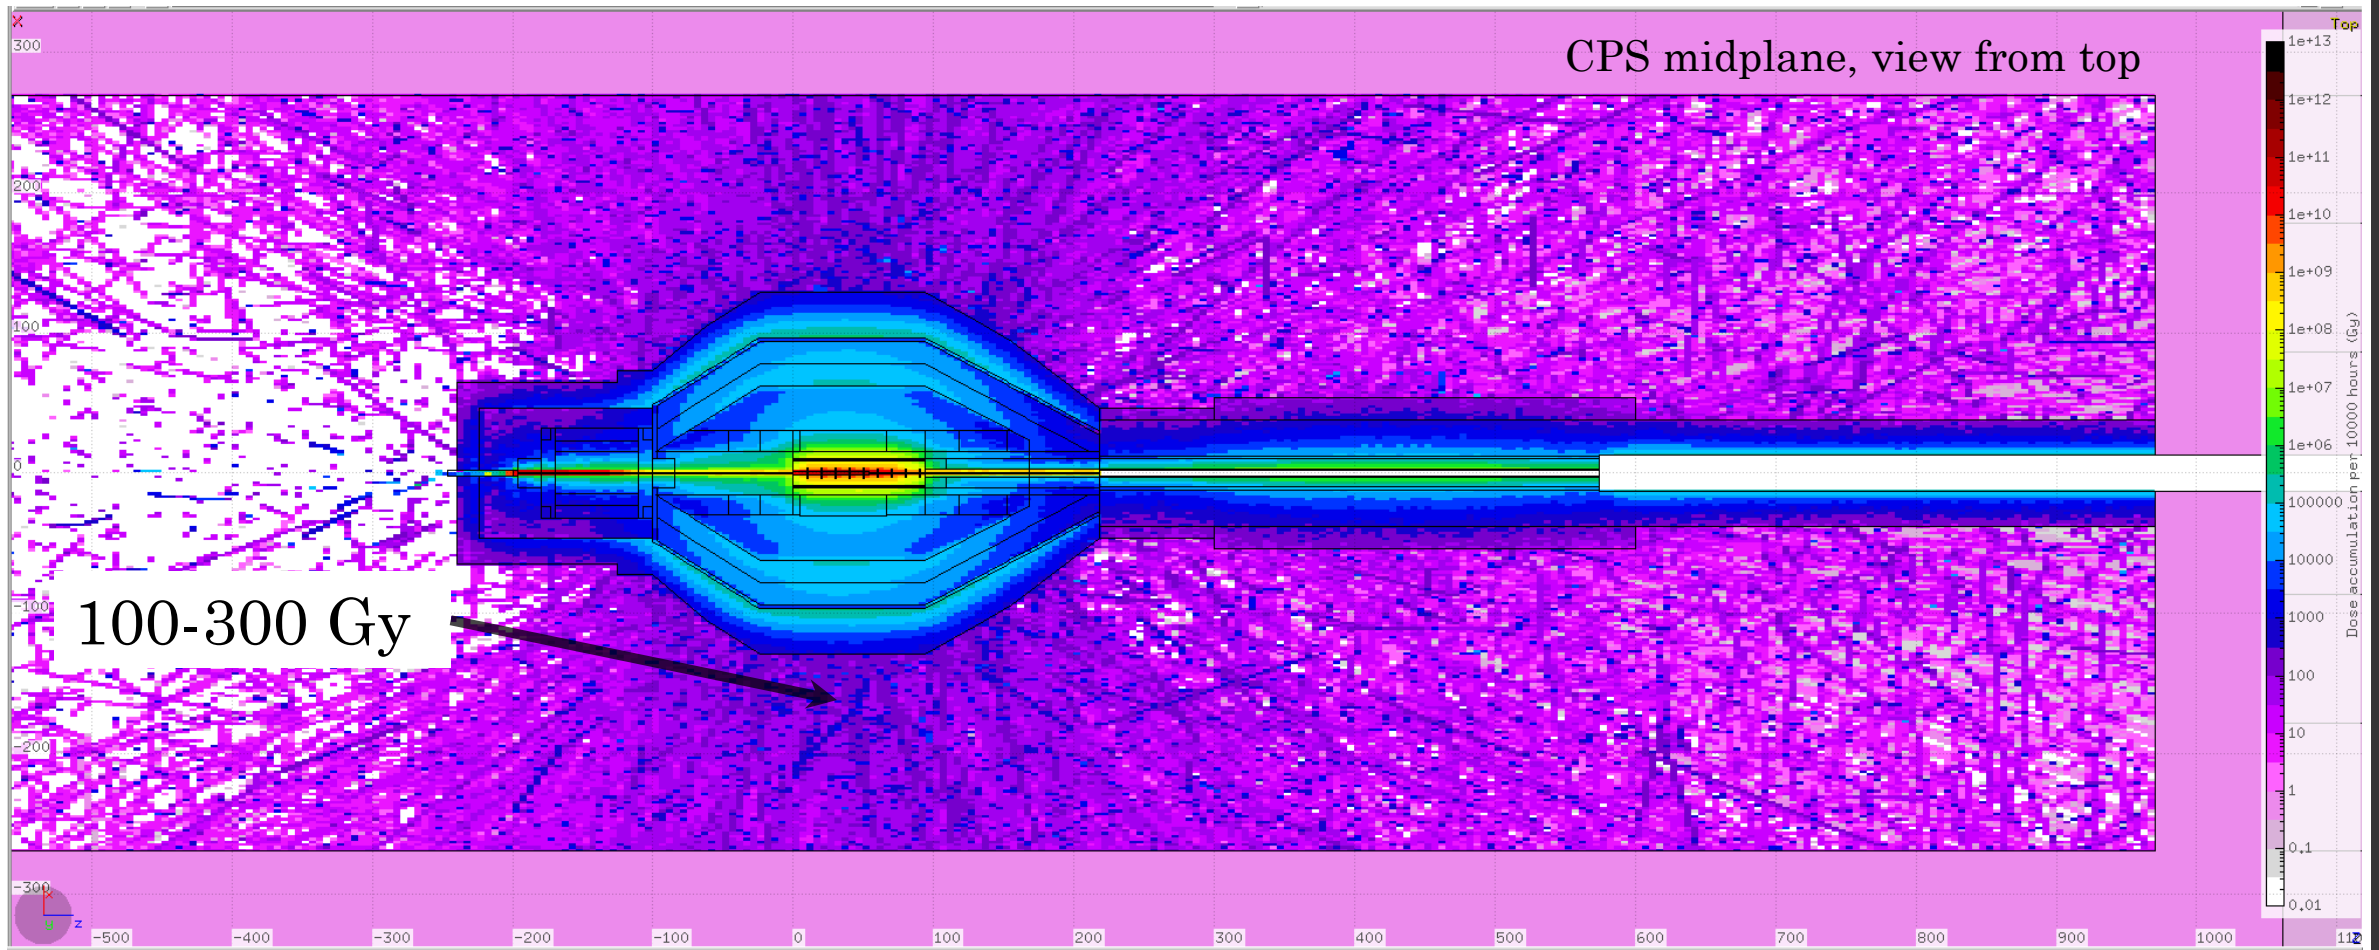


Accumulated Doses in the Magnets

- Accumulated dose to upstream magnet coils in 10000 hours is expected to be 3×10^4 Gy.
 - ❑ Magnet coil insulation made of cyanate ester resins can handle over 10^6 Gy dose.
 - Reference: P.E. Fabian, et al “Novel Radiation-Resistant Insulation Systems for Fusion Magnets,” Fusion Engineering and Design, Vol. 61-62, pp. 795-799, 2002

- Accumulated dose in the permanent magnet in 10000 hours is expected to be on the level $\sim 10^7$ Gy.
 - ❑ Hall D strontium ferrite permanent do not change at such a dose.
 - FNAL did not observe any change in B-field after a dose of 10^7 Gy.
 - FNAL gave an upper limit of 1% change, as specified in the magnet specs.

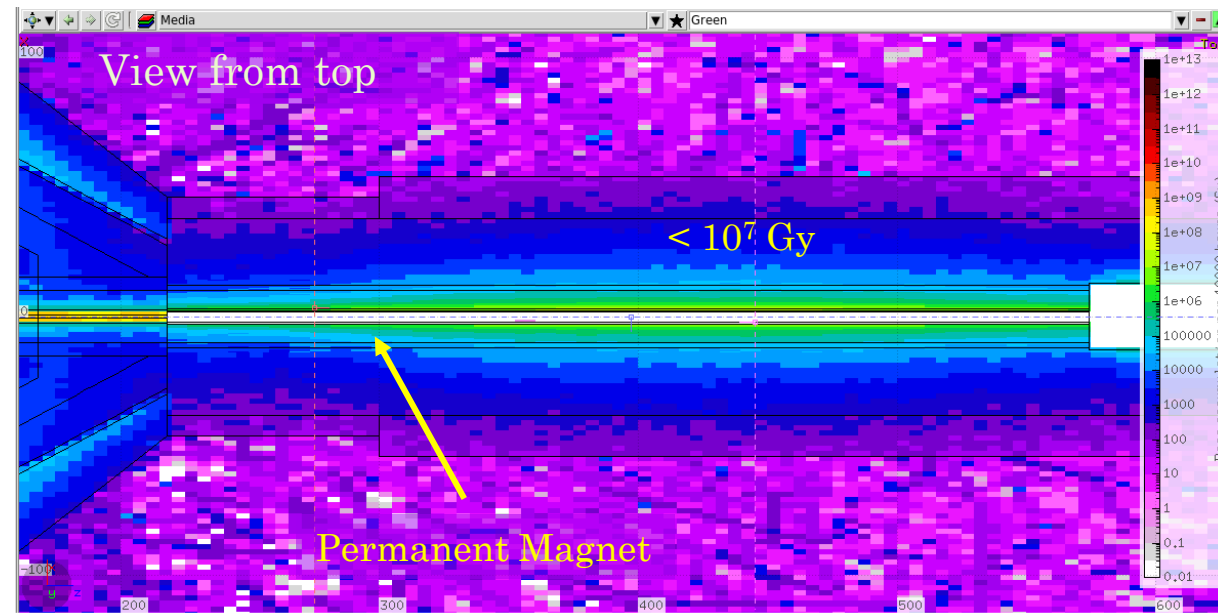
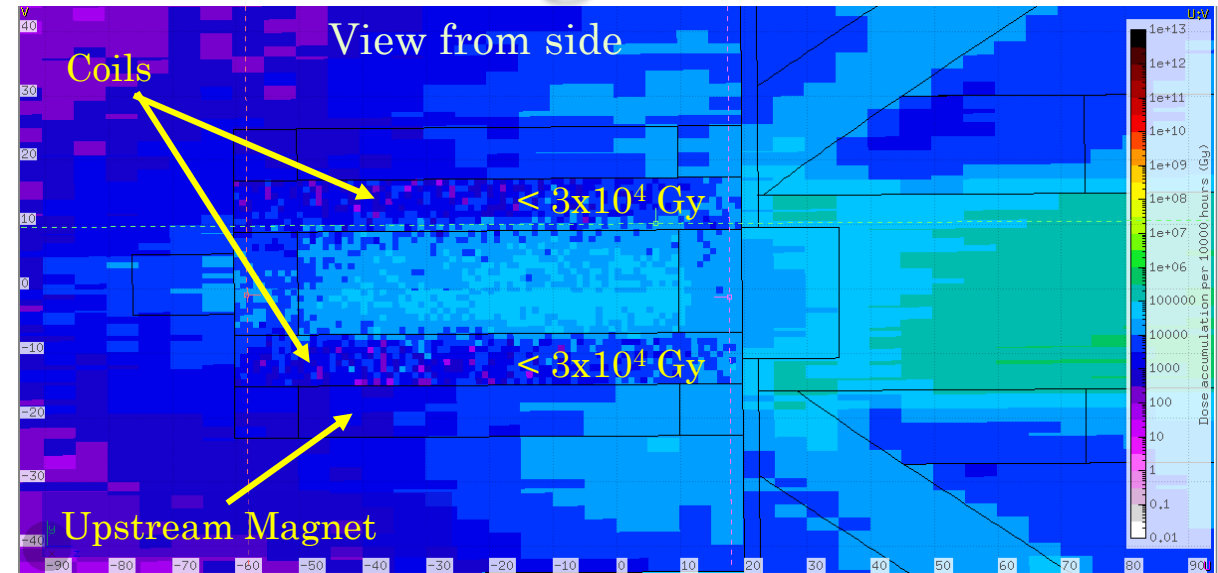


Power Deposition in the Absorber

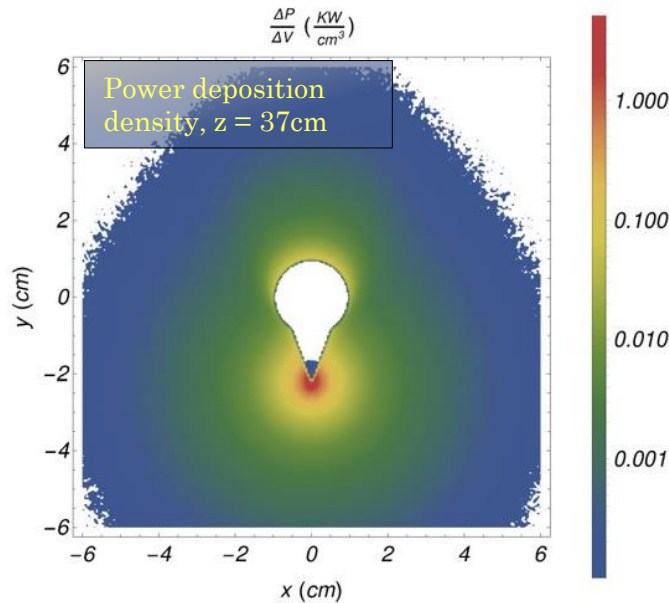

- FLUKA provides an output file with power deposition densities in 3D.
 - ❑ 30M data points inside absorber
- Almost all of the beam power (~98%) is deposited into the copper absorber.
 - ❑ Most likely that only absorber needs cooling.
 - ❑ Must prevent heat transfer from absorber to surrounding volumes.

Color indicates power deposition density (kW/cm³), x = 0 plane shown

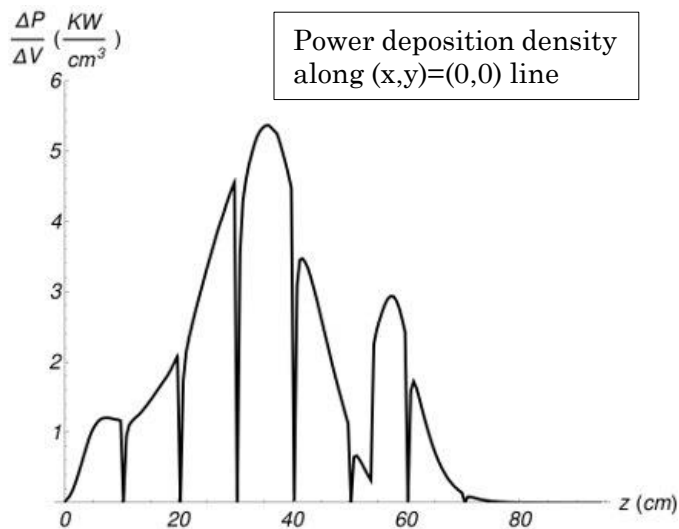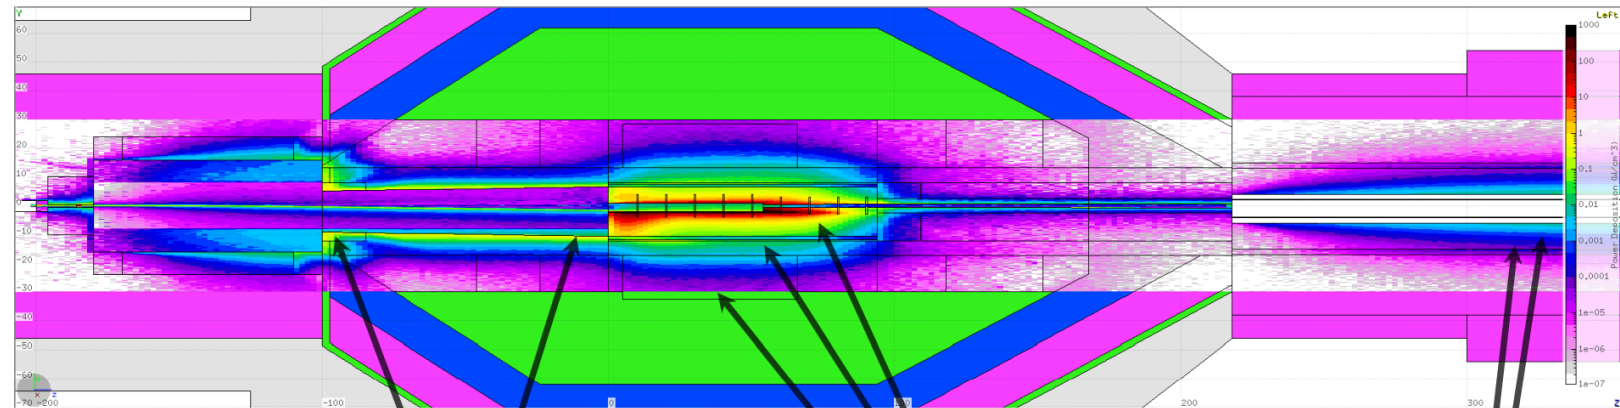

CPS Entry Collar: 34 W
 CPS Entry Iron: 156 W


Absorber: 53.545 kW
 Steel Base at Abs: 215 W
 Lead around Abs: 156 W
 Perm. Magnet Aluminum: 27 W
 Perm. Magnet Body: 20 W

Power inside CPS for 5 mA, 12 GeV beam




All other parts get less than 20 W each

Temperature

- Temperature calculations in the absorber is done using power deposition maps obtained using FLUKA.
- Two independent calculations are done by two people using two different software packages:
 - ❑ ANSYS software, popular among engineers
 - ❑ Wolfram Mathematica software, popular among scientists
 - ❑ The results are in a good agreement.
- The temperature at the hotspot is expected to be $\sim 230\text{ }^{\circ}\text{C}$ at nominal beam parameters.
- There is no high temperature at the outer boundaries of the absorber, except the front side.
 - ❑ Still need to perform ANSYS evaluation for the whole CPS.

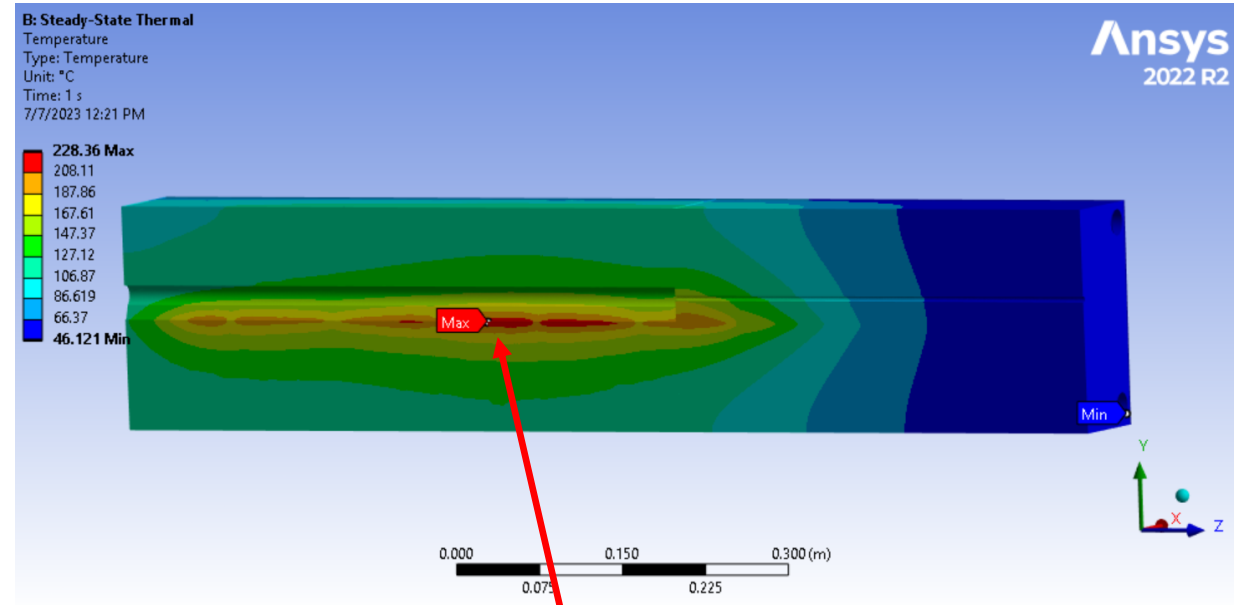


$T_{\max} \approx 230\text{ }^{\circ}\text{C}$

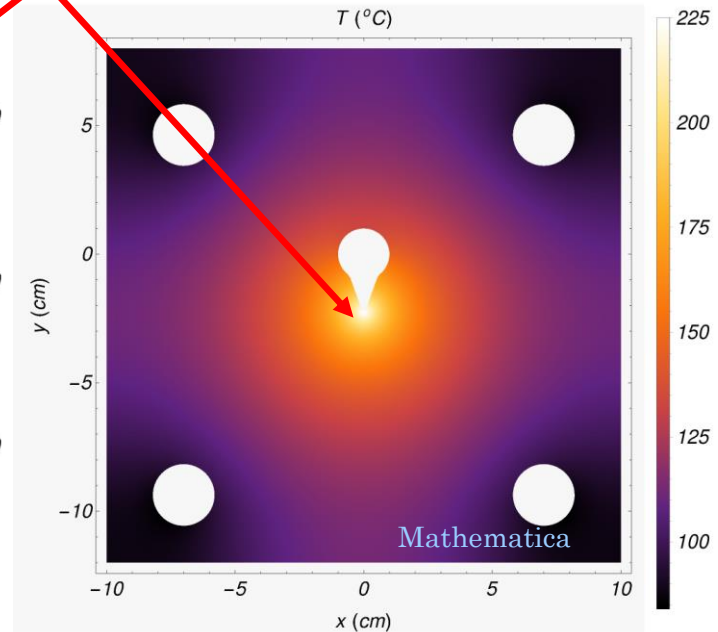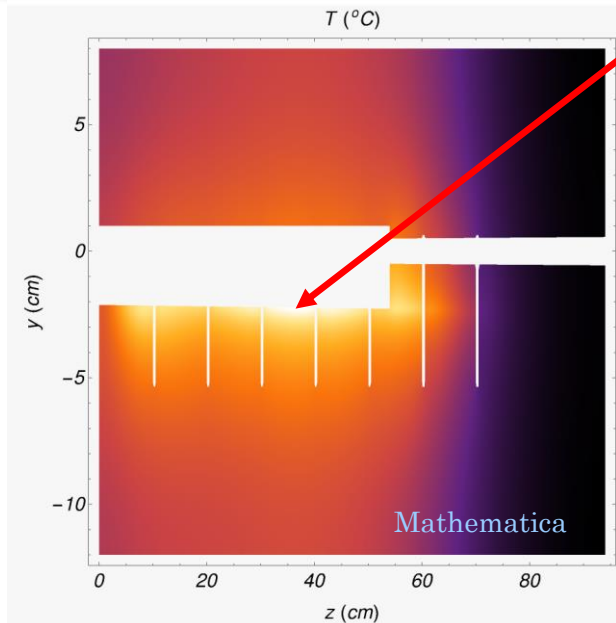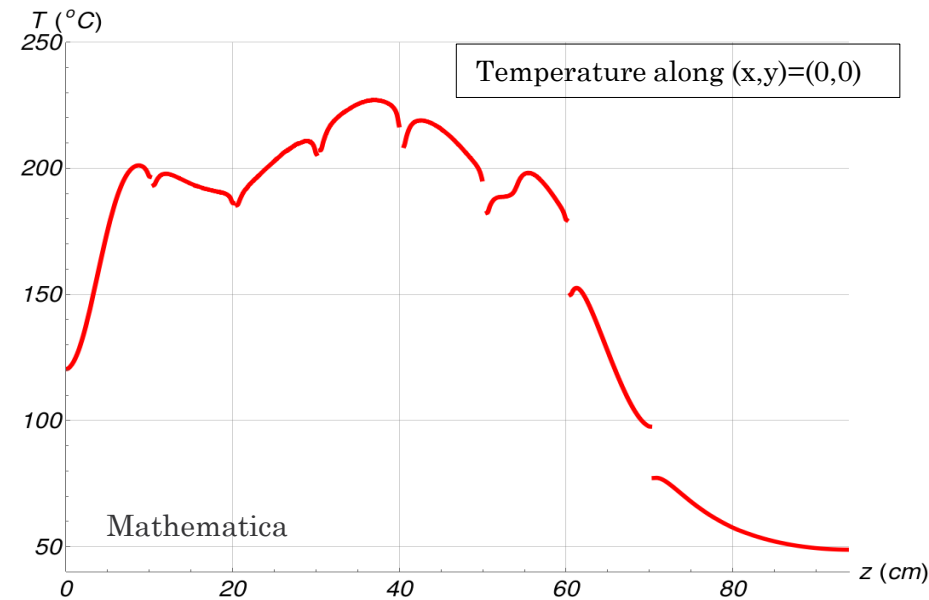

Temperature vs Beam Conditions


- Temperature in the copper core depends on the beam conditions.
- The expected temperature range is $200\text{ }^{\circ}\text{C} < T_{\text{max}} < 300\text{ }^{\circ}\text{C}$.
- Deformations and stresses are being studied in ANSYS. See talk by Tim Whitlatch.
- Multiple beam conditions has been simulated with FLUKA and the resulting temperature distributions evaluated.
- Temperatures in all studied conditions appear to be manageable.
 - ❑ We will impose restrictions on the beam conditions.

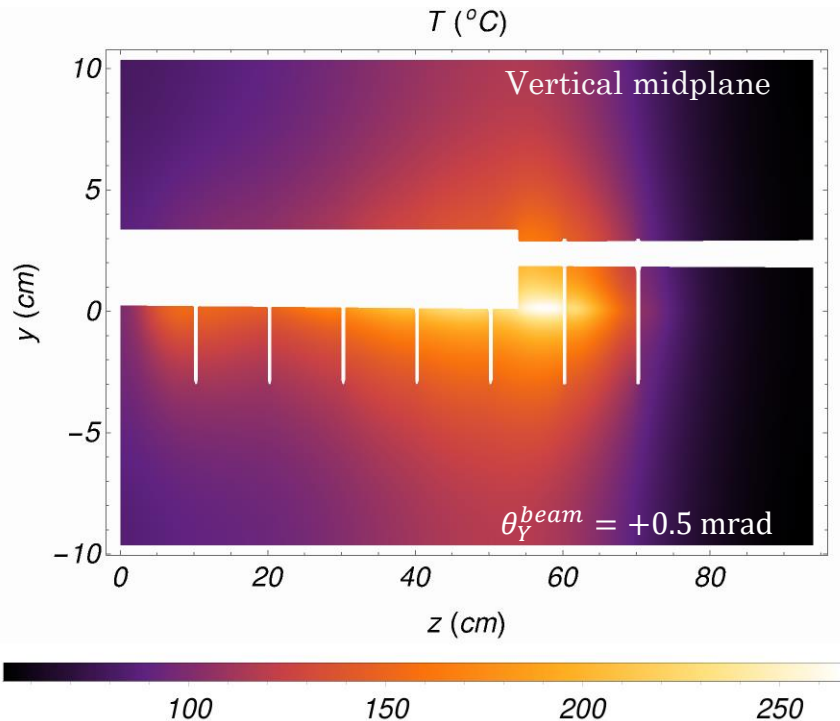


Test Configuration Name	Z_{max} (cm)	T_{max} ($^{\circ}\text{C}$)	T_{cold} ($^{\circ}\text{C}$)
All Nominal	37	230	100
$\sigma^{(x,y)}_{\text{beam}} = 0.33\text{ mm}$	43	290	105
$\sigma^{(x,y)}_{\text{beam}} = 1.5\text{ mm}$	8.5	245	100
97% B-field	56.5	245	100
103% B-field	33	240	100
-1mm shift in Y	8	265	110
+1mm shift in Y	57	265	105
-0.5mrad angle in Y	8.5	265	110
+0.5mrad angle in Y	58	275	105
+1mm shift in X	8.2	260	100
+0.5mrad angle in X	8	260	100

Electron Beam Requirements

- It is important to have a good beam on the radiator.
 - ❑ Excessive radiation in Tagger Hall.
 - ❑ Higher Temperatures in the absorber.
- We found that beam rastering will not be necessary.
 - ❑ We will need to make sure that beam profile is wide using wire scans at CPS.
- Install a girder just upstream of CPS with:
 - ❑ BCM to measure the beam current,
 - ❑ BPM to measure beam positions,
 - ❑ Wire scanner for beam widths.
- FSD trips on
 - ❑ Large electron beam positions excursions,
 - Use a collar and ion chambers.
 - ❑ Electron beam angle excursion,
 - Measure photon beam position at KPT.
 - ❑ Magnet current deviations.
 - Use power supply ADCs.
- Keep Hall D radiator scanner for the halo measurement.

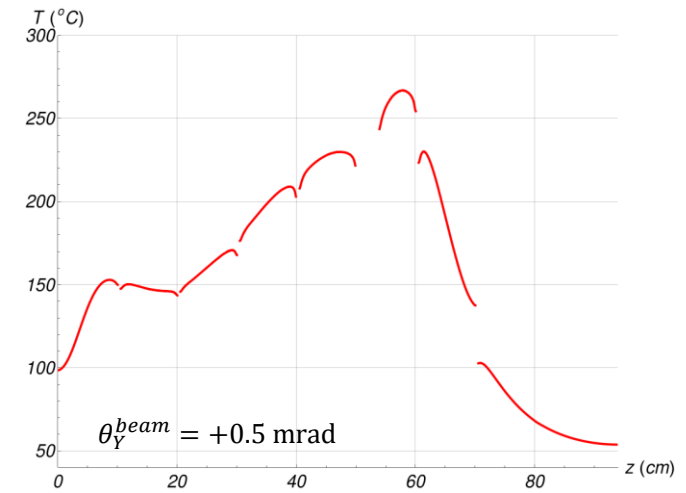

Parameter	@ CPS Radiator	@ KPT
Beam Current	$50 \text{ nA} \leq I_B \leq 5 \text{ }\mu\text{A}$	N/A
Beam Size	$0.5 \text{ mm} \leq \sigma \leq 1.5 \text{ mm}$	$\sigma \leq 1 \text{ cm}$
Beam stability (@ 1 Hz)	$\sigma \leq 0.2 \text{ mm}$	$\sigma \leq 2 \text{ mm}$
FSD is tripped at	$ \Delta x > 1 \text{ mm}$ or $ \Delta y > 1 \text{ mm}$	$ \Delta x > 1 \text{ cm}$ or $ \Delta y > 1 \text{ cm}$
Beam halo (halo-to-peak)	$< 10^{-4}$ at $r > 5\sigma$	N/A

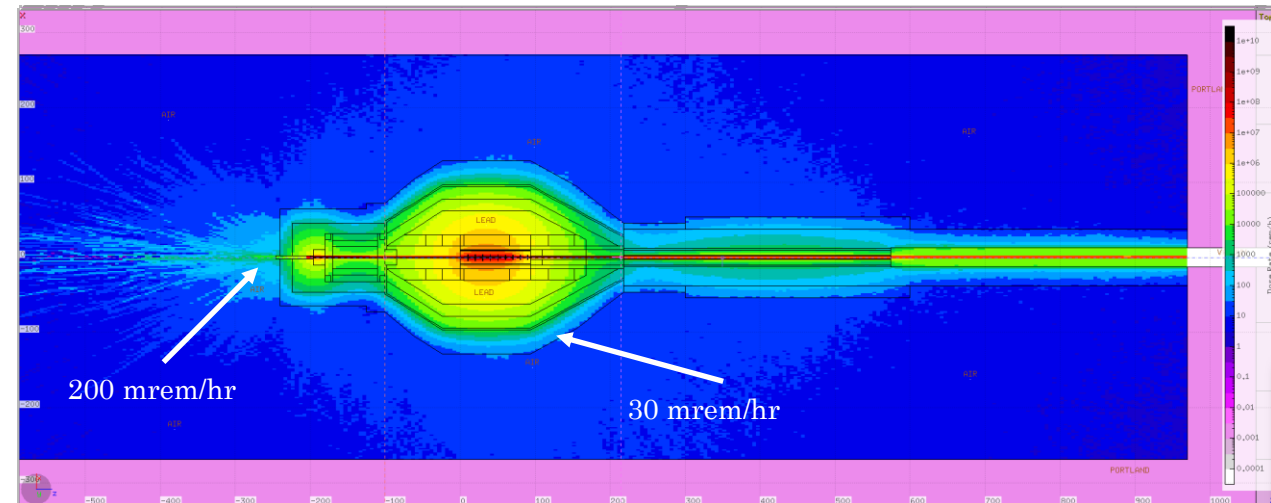



Summary

- We developed a conceptual design of CPS for Hall D.
 - ❑ It will provide photon beam at KPT that would meet KLF requirements.
 - ❑ We will use a movable platform to be able to restore GlueX beamline.
- No major R&D is required for the design and construction of CPS.
 - ❑ Need to optimize CPS and develop engineering design.
- We performed FLUKA simulation to estimate the radiation levels around CPS.
 - ❑ Radiation environment should be similar or better than GlueX would have at 5mA.
 - ❑ No civil construction is needed in tagger hall.
- We are in contact with Accelerator Division regarding beam requirements for CPS.
 - ❑ No show-stoppers are identified.
- Working on optimization of the basic design.
- Engineering design is the next step.



Potential Problems and Mitigations

- At very large vertical angles ($500 \mu\text{rad}$), the beam can penetrate deep into CPS and cause somewhat elevated temperatures ($275 \text{ }^\circ\text{C}$).
 - ❑ The radiation environment is probably not going to be affected much.
 - ❑ The photon beam position needs to be monitored and used in the beam interlock.
- At large horizontal shifts ($\sim 1 \text{ mm}$), the beam can impact the upstream wall of the absorber missing the keyhole and thus cause high temperatures ($300 \text{ }^\circ\text{C}$).
 - ❑ The radiation environment is probably not going to be affected much.
 - ❑ Beam position need to be monitored and beam needs to be shut off at large excursions.

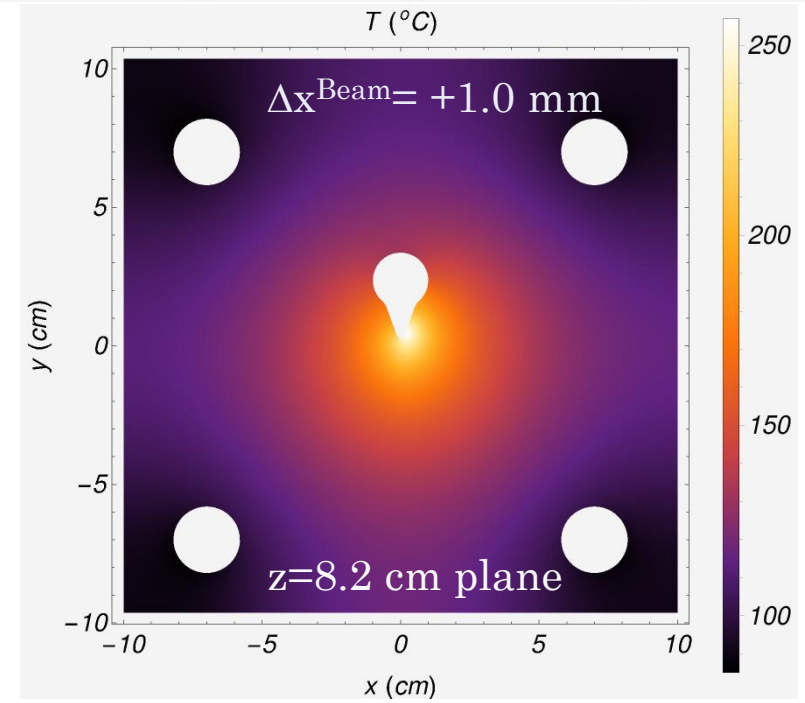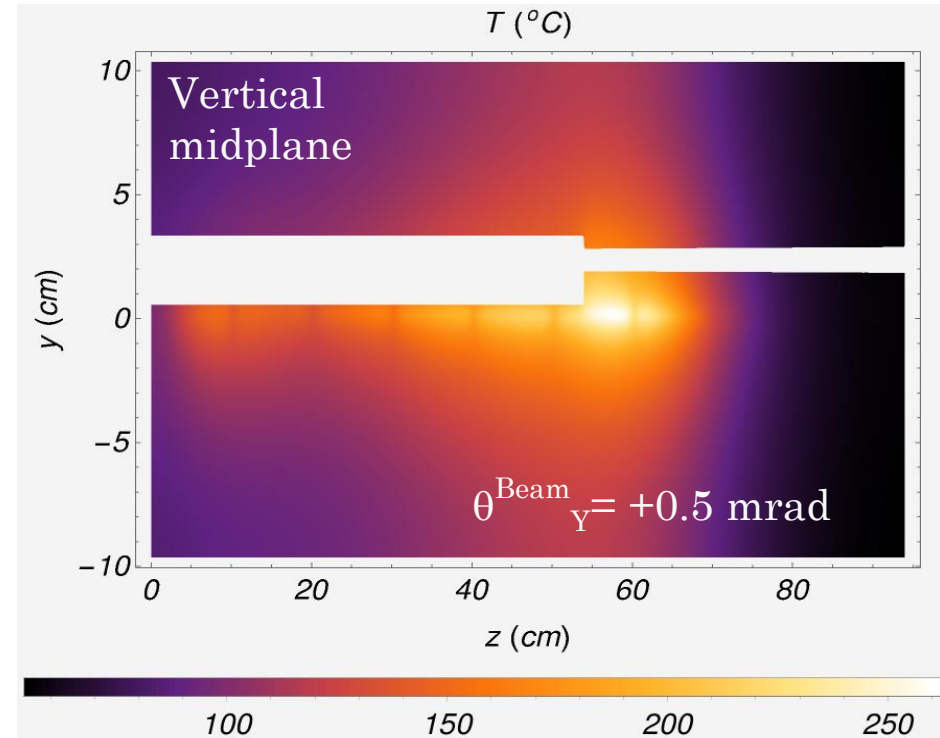

Cost and Schedule


- The total weight estimate for the new installations in Tagger Hall is ~90??? metric tons.
 - ❑ According to Facilities Management, Tagger Hall can easily accommodate 100 metric tons.
- Total cost of the CPS, including magnet and PS, is ~\$1M.
 - ❑ Electron beam instrumentations upstream of CPS will be extra.




CPS Location in Tagger Hall



➤ Probably not needed

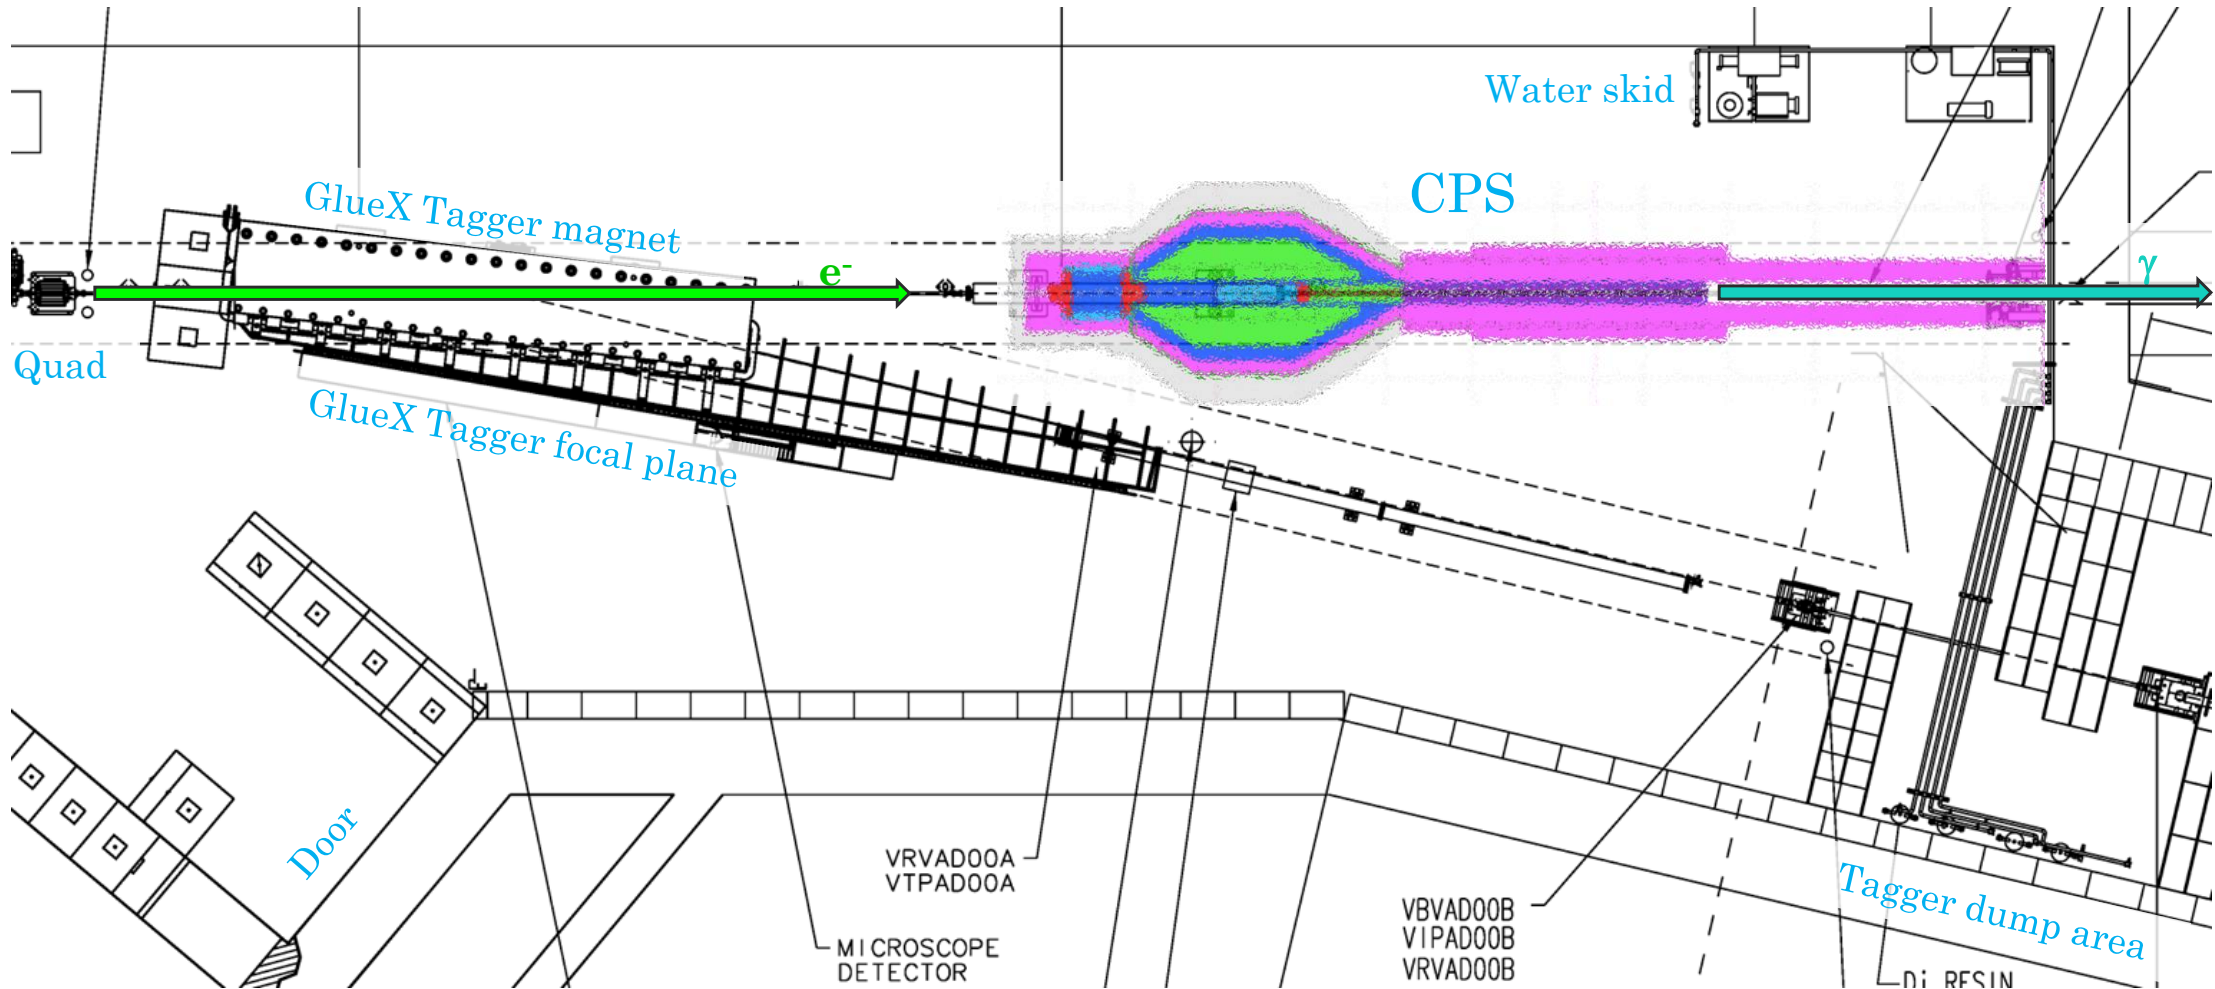

➤ fsgfd

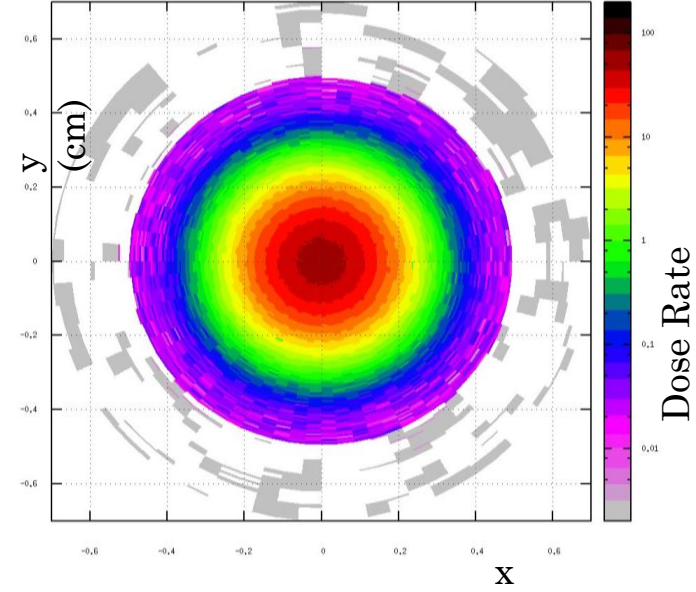

8/2/2023

KLF ERR-1 Review

Hovanes Egiyan

Grem / hr